


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL092418\
Data File : VL032513.D
Acq On : 24 Sep 2018 15:48
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092418AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Sep 25 05:17:15 2018
Last Update : Tue Sep 25 05:17:15 2018

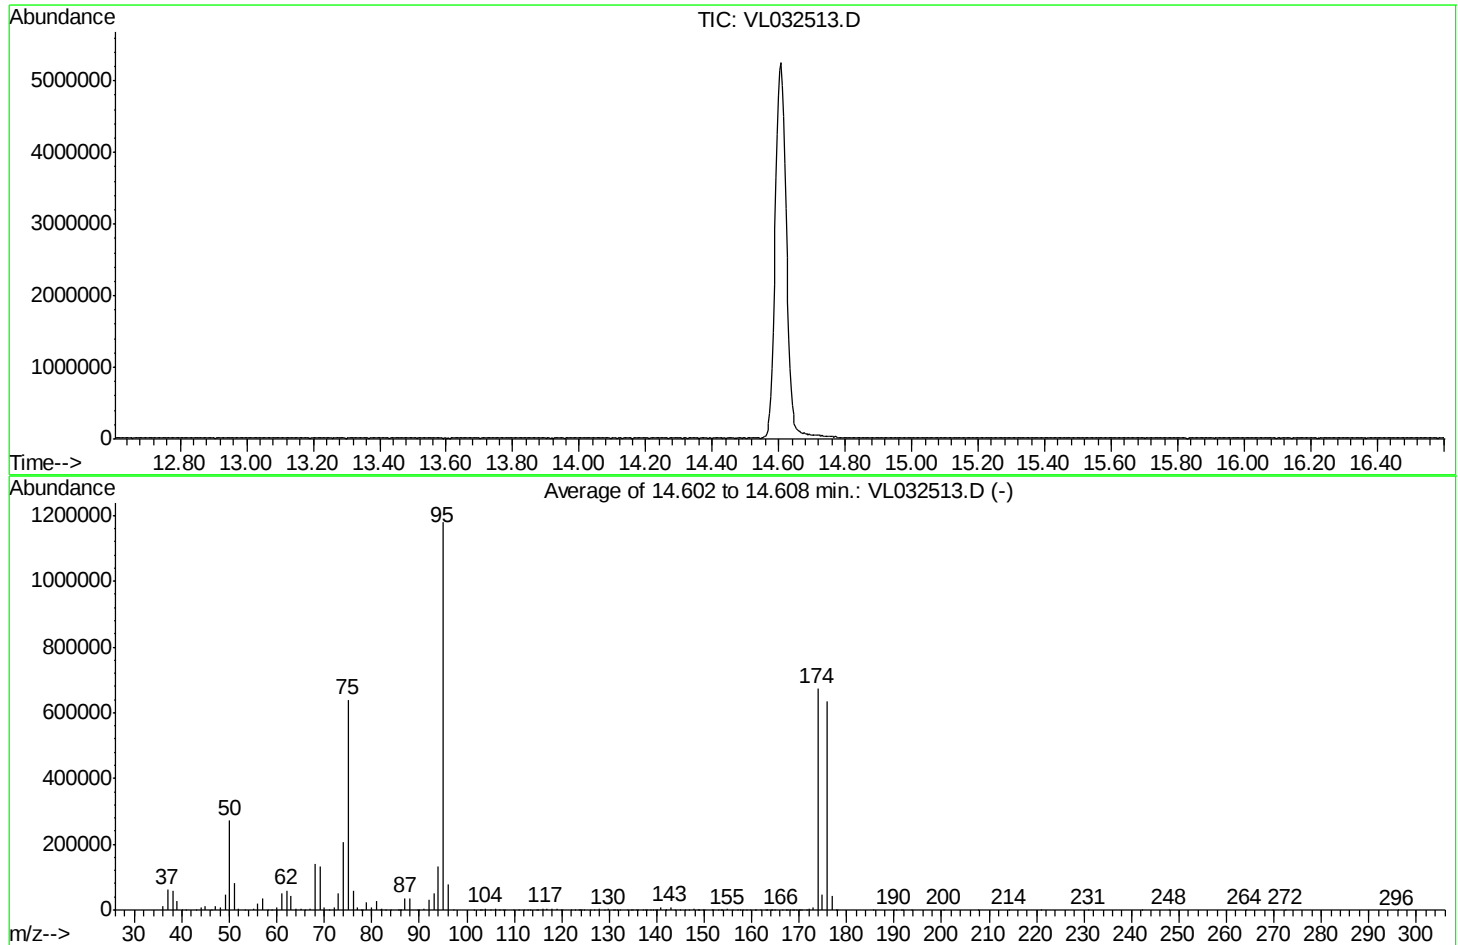

AutoFind: Scans 3628, 3629, 3630; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	270805	PASS
75	95	30	66	54.2	639253	PASS
95	95	100	100	100.0	1179306	PASS
96	95	5	9	6.7	79210	PASS
173	174	0.00	2	1.1	7177	PASS
174	95	50	120	57.0	672448	PASS
175	174	4	9	7.1	47560	PASS
176	174	93	101	94.3	633834	PASS
177	176	5	9	6.7	42682	PASS