

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL092718\
Data File : VL032552.D
Acq On : 27 Sep 2018 16:29
Operator : SY/AP
Sample : QC091218 CAN 10282
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC091218 CAN 10282

Quant Time: Sep 29 22:59:07 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092418AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Sep 25 05:17:15 2018
QLast Update : Tue Sep 25 05:17:15 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.79	49	1386345	10.00	ppbv	-0.02
33) 1,4-Difluorobenzene	7.32	114	3163633	10.00	ppbv	-0.03
55) Chlorobenzene-d5	12.27	117	3258648	10.00	ppbv	-0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.61	95	2251953	9.16	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	91.60%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL092718\
Data File : VL032552.D
Acq On : 27 Sep 2018 16:29
Operator : SY/AP
Sample : QC091218 CAN 10282
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC091218 CAN 10282

Quant Time: Sep 29 22:59:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL092418AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Sep 25 05:17:15 2018
QLast Update : Tue Sep 25 05:17:15 2018
Response via : Initial Calibration

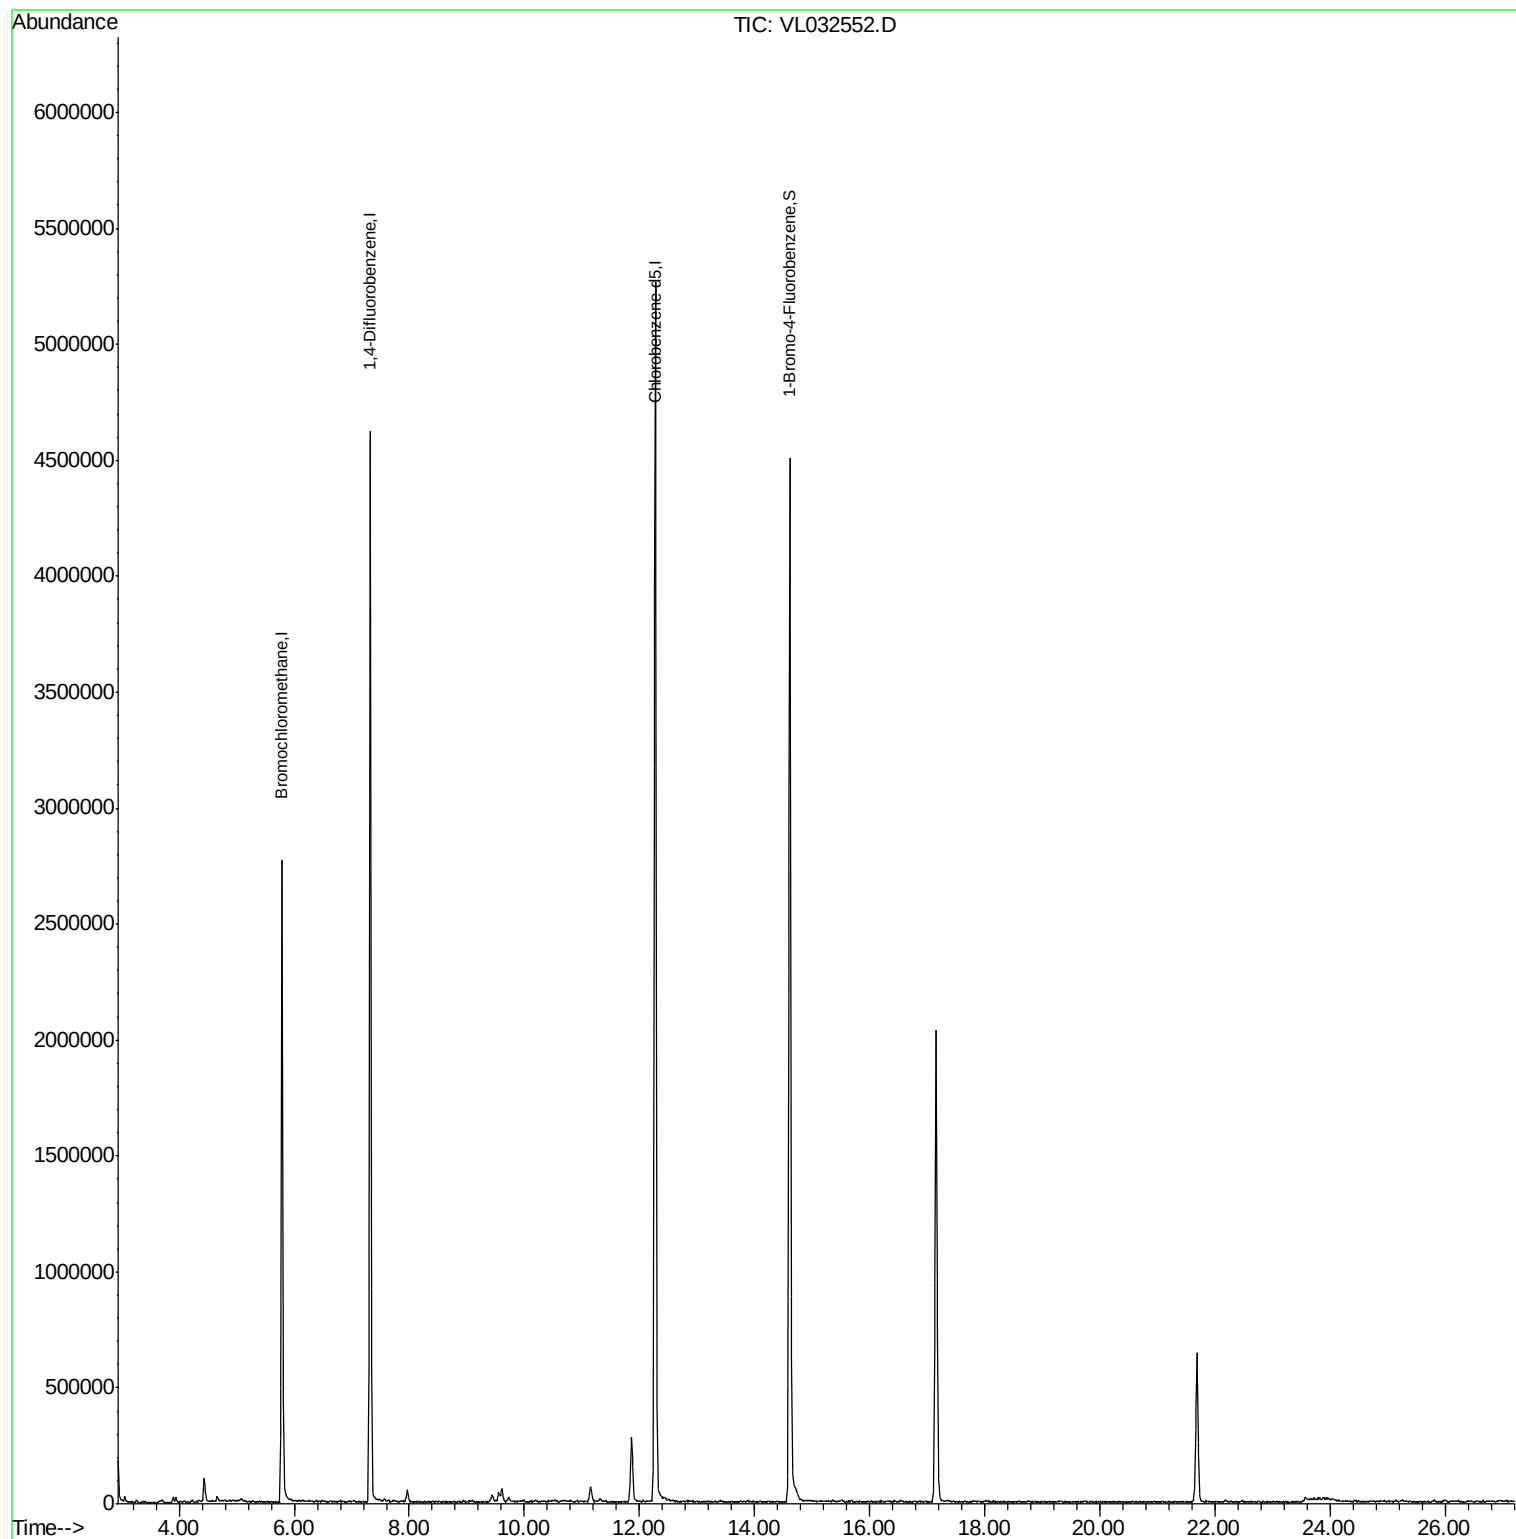

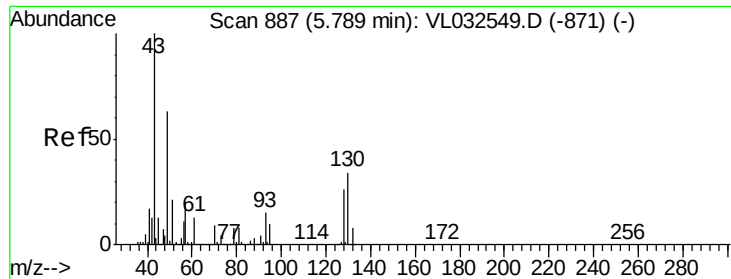

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.79 min Scan# 886

Delta R.T. -0.02 min

Lab File: VL032552.D

Acq: 27 Sep 2018 16:29

Instrument :

MSVOA_L

ClientSampleId :

QC091218 CAN 10282


Tgt Ion: 49 Resp: 1386345

Ion Ratio Lower Upper

49 100

128 43.4 20.7 62.1




130 55.7 26.6 79.7

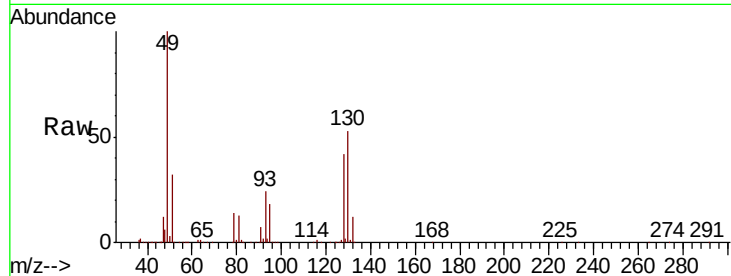

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

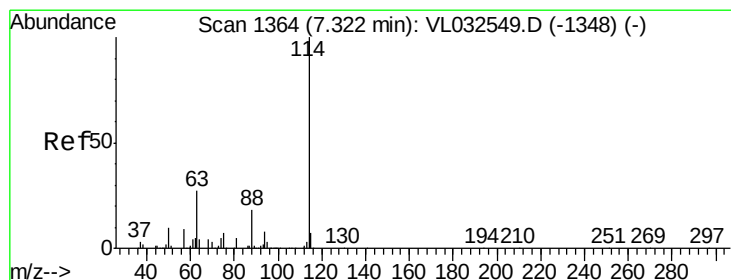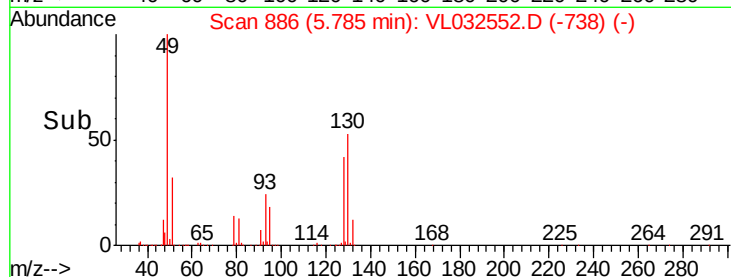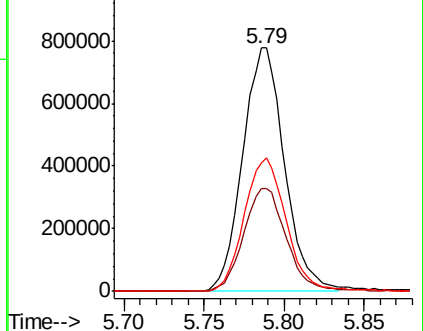

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.32 min Scan# 1363

Delta R.T. -0.03 min

Lab File: VL032552.D

Acq: 27 Sep 2018 16:29


Tgt Ion: 114 Resp: 3163633

Ion Ratio Lower Upper

114 100

63 27.8 22.2 33.4



88 18.6 15.0 22.4

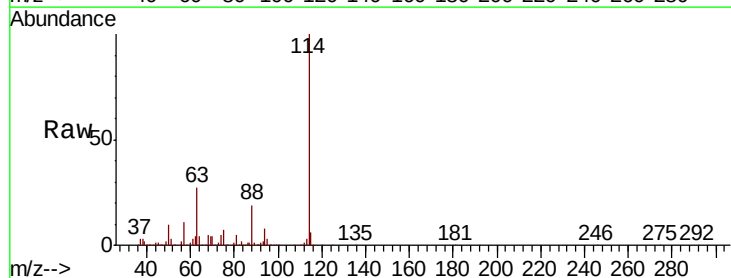


Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

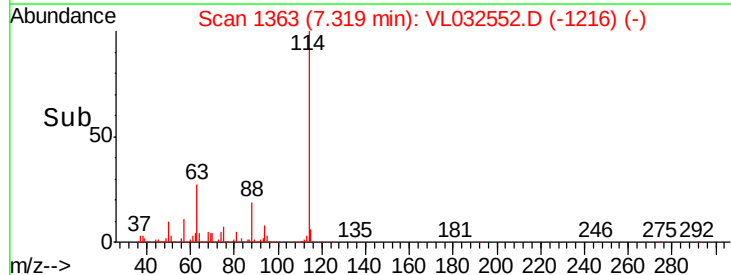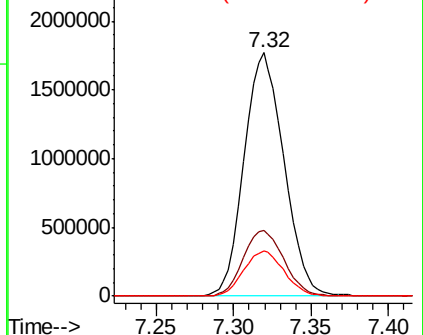

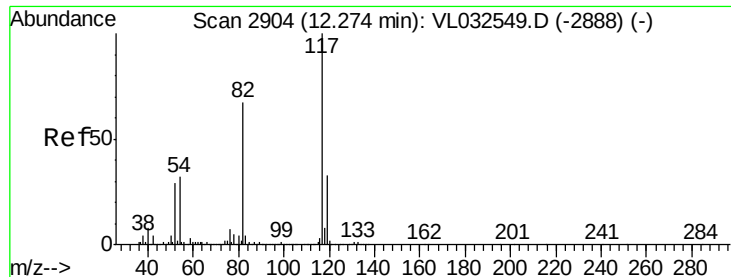

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.27 min Scan# 2903

Delta R.T. -0.03 min

Lab File: VL032552.D

Acq: 27 Sep 2018 16:29

Instrument :

MSVOA_L

ClientSampleId :

QC091218 CAN 10282


Tgt Ion: 117 Resp: 3258648

Ion Ratio Lower Upper

117 100

82 67.5 53.0 79.6




119 32.6 45.9 68.9#

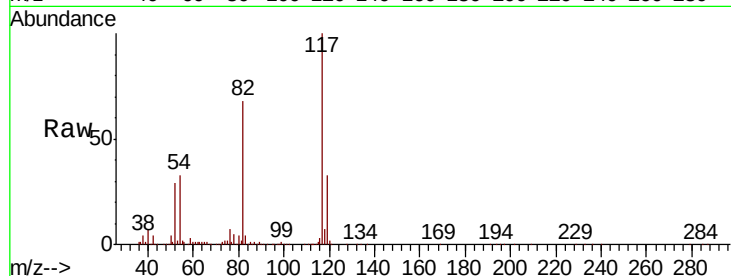

Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

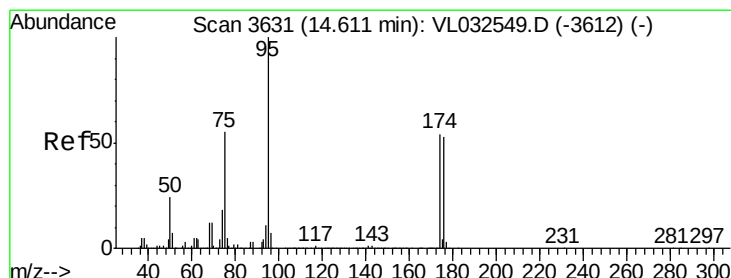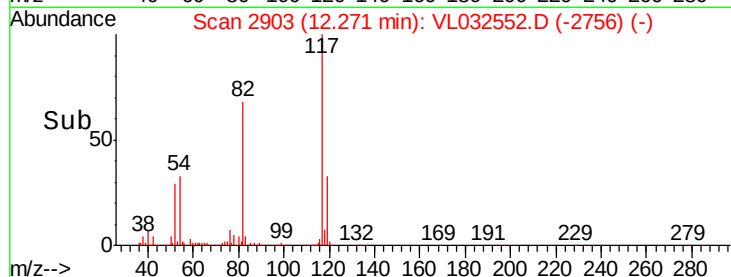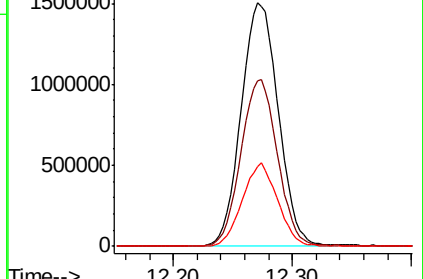

#68

1-Bromo-4-Fluorobenzene

Concen: 9.164 ppbv

RT: 14.61 min Scan# 3631

Delta R.T. -0.02 min

Lab File: VL032552.D

Acq: 27 Sep 2018 16:29


Tgt Ion: 95 Resp: 2251953

Ion Ratio Lower Upper

95 100

174 58.8 46.3 69.5

175 4.3 3.4 5.0

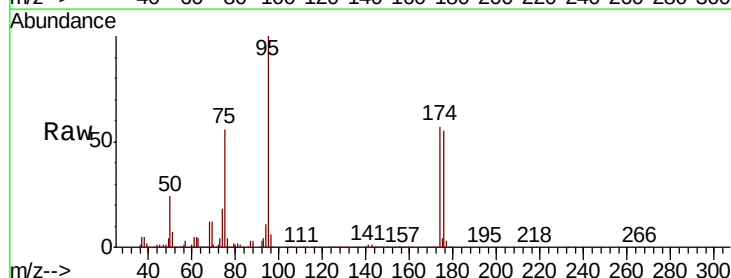

Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

