


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092718\
Data File : VL032548.D
Acq On : 27 Sep 2018 12:29
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092418AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Sep 25 05:17:15 2018
Last Update : Tue Sep 25 05:17:15 2018

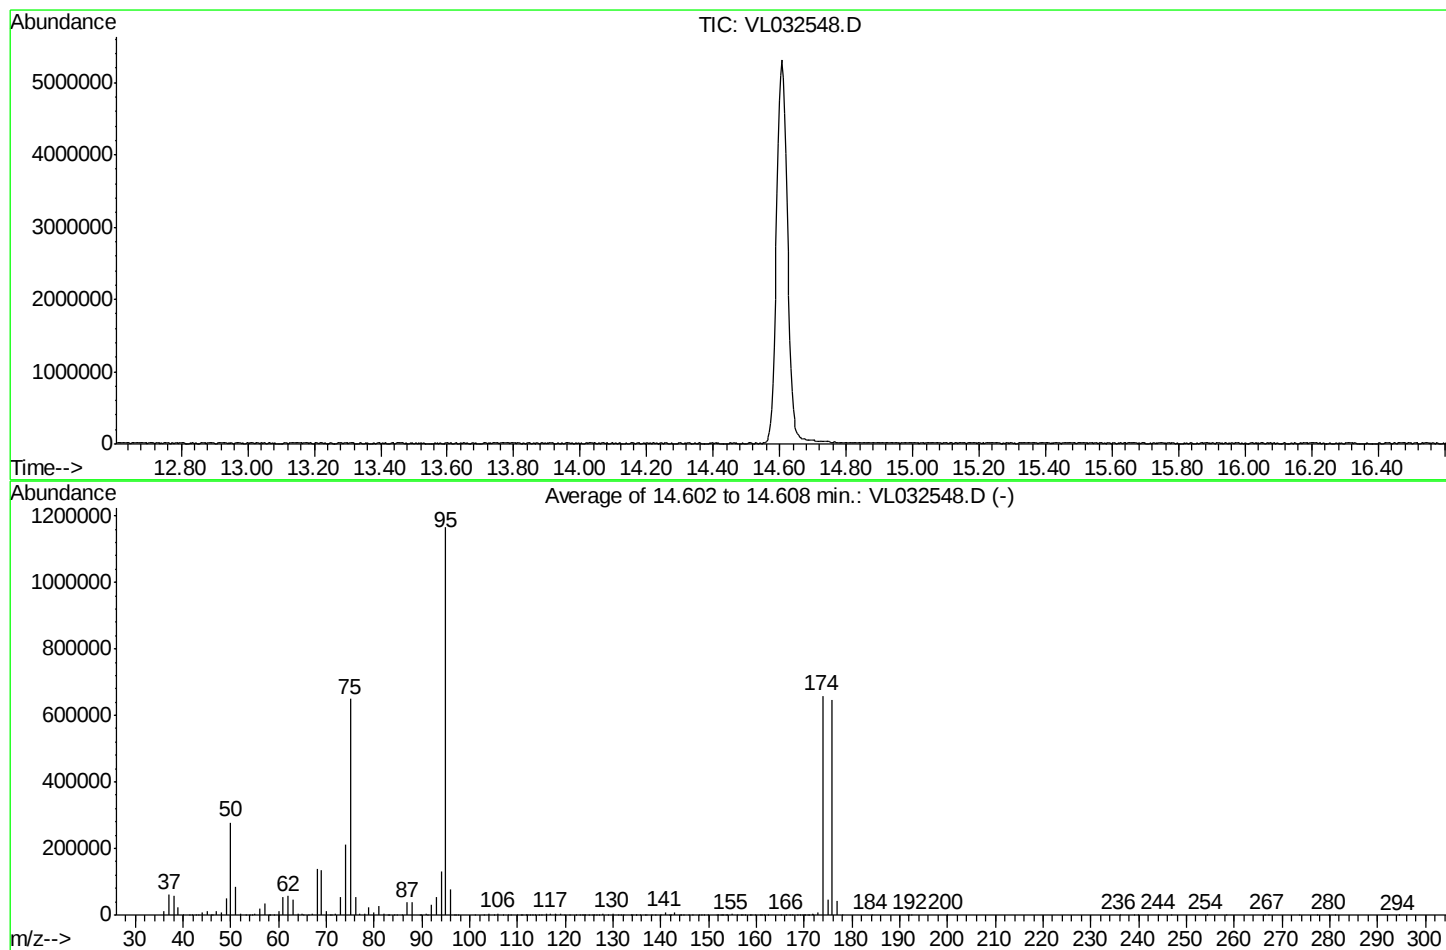

AutoFind: Scans 3628, 3629, 3630; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	278933	PASS
75	95	30	66	55.7	649130	PASS
95	95	100	100	100.0	1165312	PASS
96	95	5	9	6.6	77029	PASS
173	174	0.00	2	1.1	7213	PASS
174	95	50	120	56.6	659754	PASS
175	174	4	9	7.2	47792	PASS
176	174	93	101	97.7	644736	PASS
177	176	5	9	6.3	40808	PASS