


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL092721\
 Data File : VL037671.D
 Acq On : 27 Sep 2021 8:30
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021
 Last Update : Thu Sep 16 13:42:46 2021

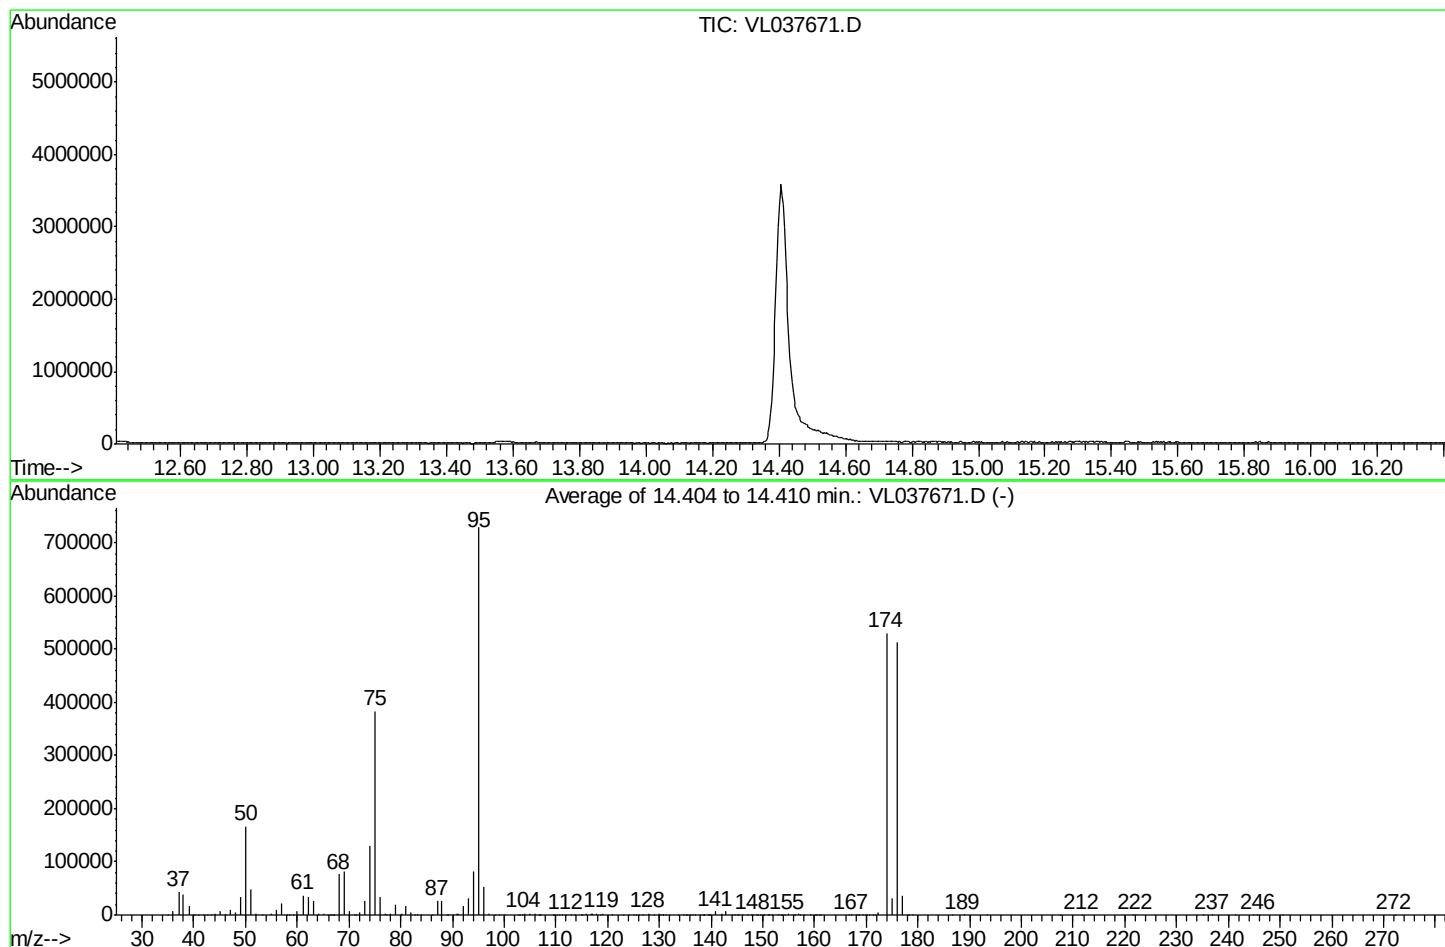

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	167040	PASS
75	95	30	66	52.6	383232	PASS
95	95	100	100	100.0	729194	PASS
96	95	5	9	7.3	52949	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.8	530837	PASS
175	174	4	9	5.9	31192	PASS
176	174	93	101	96.5	512000	PASS
177	176	5	9	6.9	35096	PASS