
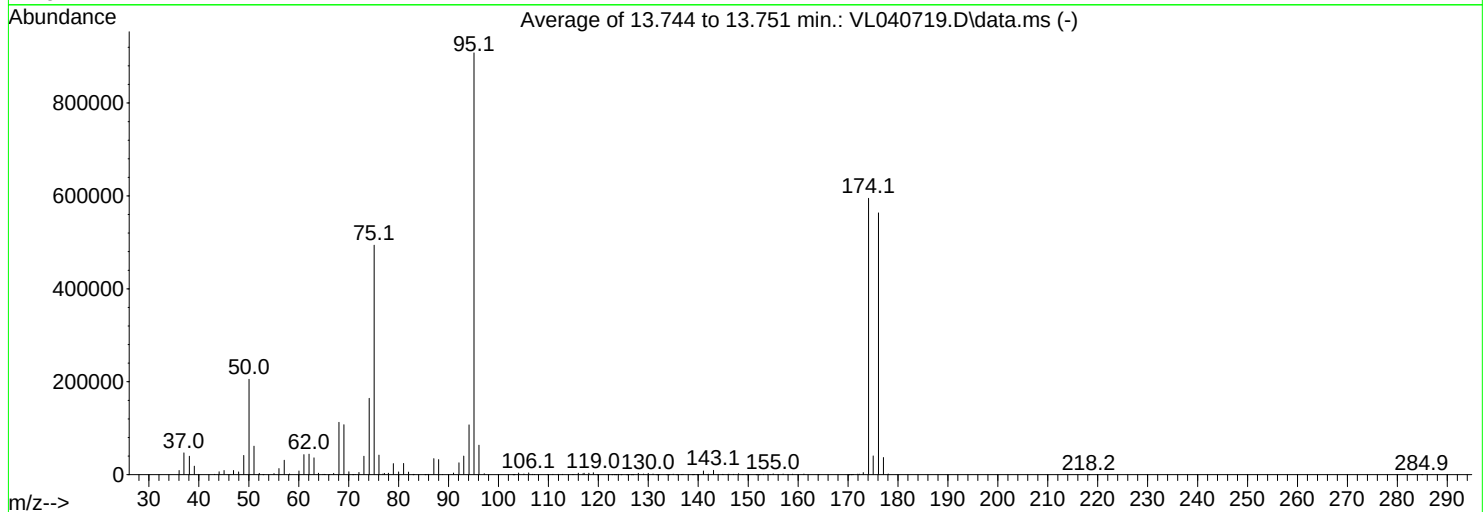


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092723\
Data File : VL040719.D
Acq On : 27 Sep 2023 8:19
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091423AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 19 05:12:43 2023

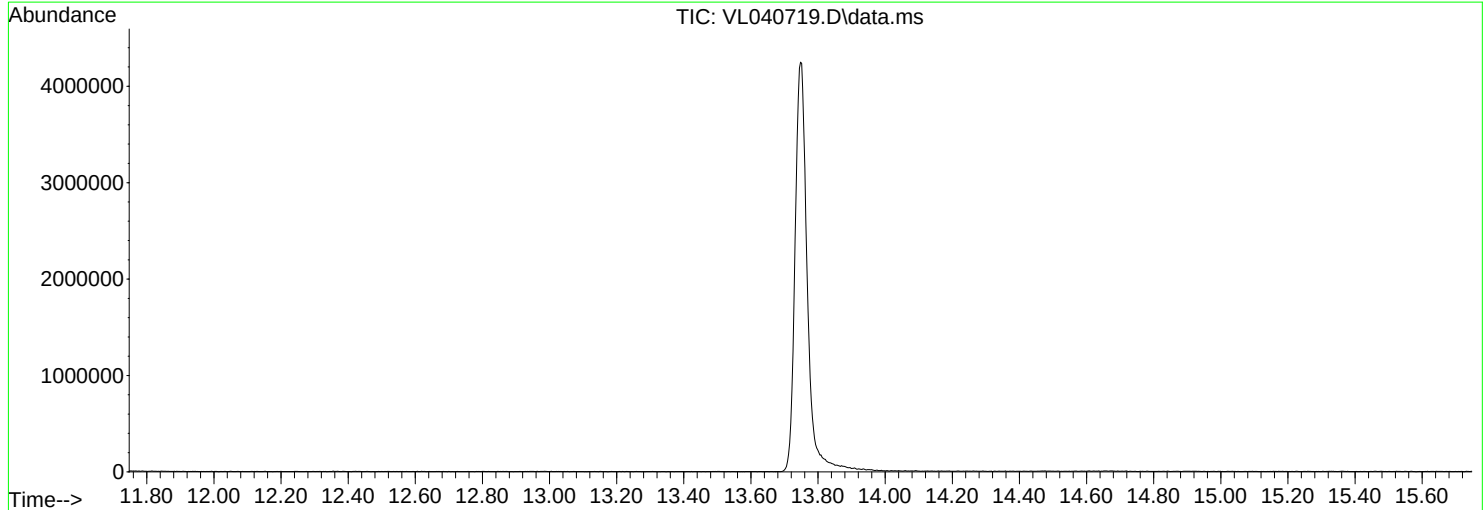

AutoFind: Scans 3465, 3466, 3467; Background Corrected with Scan 3441

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.6	205205	PASS
75	95	30	66	54.4	493845	PASS
95	95	100	100	100.0	908011	PASS
96	95	5	9	7.0	63245	PASS
173	174	0.00	2	0.8	4496	PASS
174	95	50	120	65.5	594987	PASS
175	174	4	9	6.8	40365	PASS
176	174	93	101	94.7	563648	PASS
177	176	5	9	6.5	36789	PASS

Average of 13.744 to 13.751 min.: VL040719.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9071	47.95	5992	61.05	43085	70.05	6251
37.00	46755	49.00	41291	62.05	44205	70.80	111
38.10	39648	50.05	205205	63.05	36184	71.30	21
39.10	18160	51.05	61309	63.95	3067	72.05	485
40.00	579	52.10	2852	64.85	819	73.05	39459
43.15	674	52.85	120	65.10	590	74.10	164480
44.05	6336	55.05	2449	65.30	284	75.10	493845
45.05	9115	56.05	13083	66.15	333	76.05	42200
45.85	487	57.10	30912	67.00	2849	76.85	1542
46.20	299	58.15	1362	68.05	112792	77.15	2917
46.95	8943	60.05	7962	69.05	107579	77.95	3024

Average of 13.744 to 13.751 min.: VL040719.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	23896	88.80	372	105.10	1552	116.90	1816
80.00	6013	91.00	3392	106.05	3927	117.15	3266
81.00	24163	92.10	25467	106.80	664	118.10	3120
82.00	5463	93.05	39963	107.20	299	119.00	4089
82.90	121	94.10	107128	109.80	420	119.80	59
83.05	664	95.10	908011	110.90	664	121.95	143
85.30	57	96.10	63245	111.95	578	122.70	50
85.70	290	97.15	2102	112.80	633	123.20	56
86.00	740	102.90	162	114.85	467	123.50	152
87.05	34507	103.10	138	115.10	319	124.00	606
88.00	32427	104.05	3379	116.00	2962	124.55	185

Average of 13.744 to 13.751 min.: VL040719.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	108	134.10	119	142.05	940	149.95	651
126.15	479	135.00	1189	143.05	9457	151.60	77
126.60	70	135.70	144	144.00	580	151.90	349
126.90	143	136.70	332	144.85	648	152.20	168
128.00	2773	136.95	850	145.10	384	153.05	626
129.05	1464	138.85	179	145.80	493	153.90	420
130.00	2654	139.25	323	146.15	1169	154.40	280
130.95	1329	139.80	156	147.05	551	155.00	1839
131.70	105	140.00	212	148.10	1974	156.00	202
132.00	123	141.05	7921	148.95	475	157.00	1386
133.70	79	141.80	285	149.70	336	157.95	432

Average of 13.744 to 13.751 min.: VL040719.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.90	1117	174.10	594987				
161.15	1372	175.05	40365				
164.00	57	176.10	563648				
170.00	59	177.10	36789				
170.20	95	178.05	1407				
170.60	56	218.20	83				
170.85	418	284.90	57				
171.10	227						
171.95	1081						
172.25	1008						
173.05	4496						