
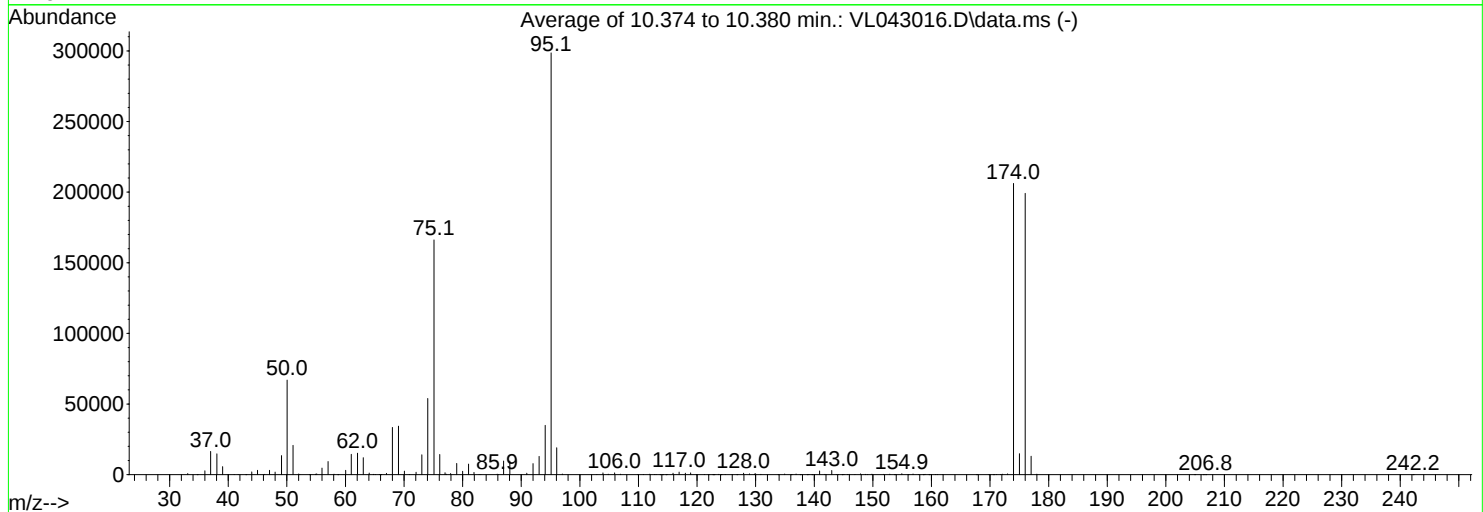


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL093025\
Data File : VL043016.D
Acq On : 30 Sep 2025 07:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL093025AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 01 00:19:41 2025

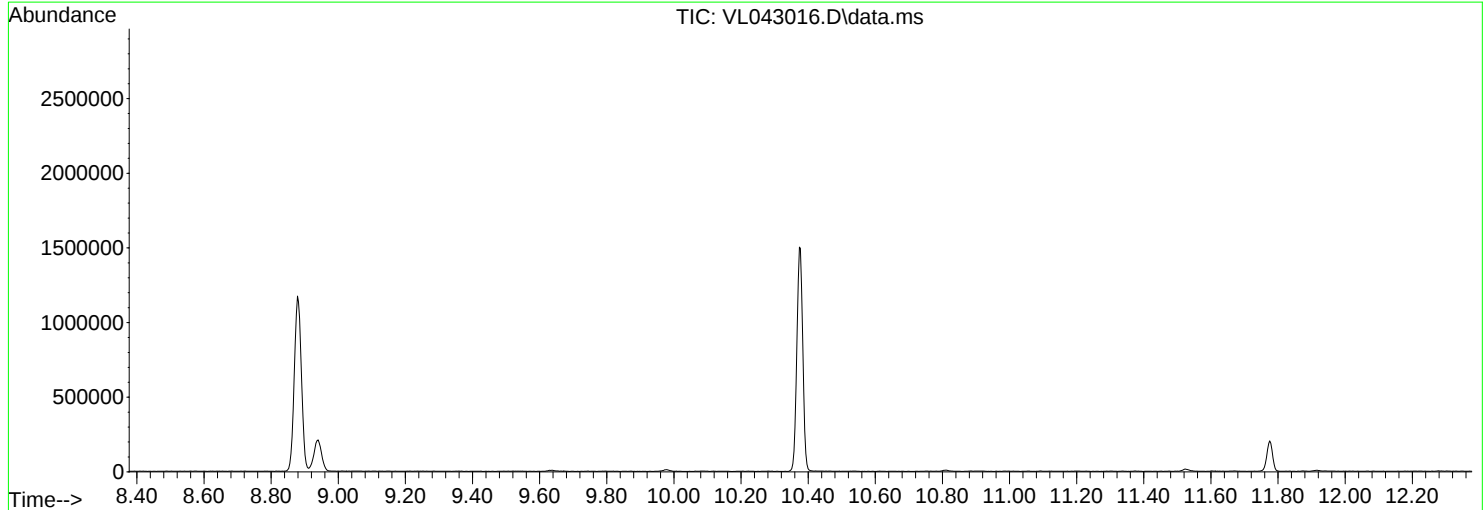

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.4	66933	PASS
75	95	30	66	55.6	166165	PASS
95	95	100	100	100.0	298624	PASS
96	95	5	9	6.4	19044	PASS
173	174	0.00	2	0.3	610	PASS
174	95	50	120	69.0	206144	PASS
175	174	4	9	7.2	14877	PASS
176	174	93	101	96.6	199189	PASS
177	176	5	9	6.5	13044	PASS

Average of 10.374 to 10.380 min.: VL043016.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	761	45.00	3054	55.10	543	65.10	61
34.70	20	46.15	241	56.00	4696	65.80	10
36.00	2676	47.05	3045	57.05	9347	66.00	4
37.00	16395	48.00	1774	58.05	372	67.00	97
38.05	14703	49.10	13521	58.70	26	68.00	33400
39.05	5726	50.05	66933	60.05	3072	69.05	34368
40.00	156	51.05	20707	61.00	14355	70.05	2468
41.00	97	52.00	510	62.05	15152	70.90	137
41.70	81	52.20	221	63.05	12061	72.05	1679
43.00	22	53.90	31	64.05	1169	73.05	14071
44.00	1954	54.90	318	64.80	201	74.05	53960

Average of 10.374 to 10.380 min.: VL043016.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	166165	85.90	301	102.90	87	114.10	43
76.10	14257	86.10	84	103.95	1255	114.70	56
77.00	1342	87.00	9625	104.85	405	114.90	68
77.20	334	88.05	9632	105.95	1214	115.90	977
77.95	848	90.95	991	106.95	320	116.95	1782
79.00	7937	92.00	7857	109.90	175	118.00	1061
80.00	2347	93.05	12945	110.85	164	118.90	1310
81.00	7494	94.10	34859	111.95	295	119.85	55
81.95	1567	95.10	298624	112.75	141	121.25	109
82.80	76	96.05	19044	113.00	97	121.90	17
83.10	117	97.00	488	113.70	17	122.70	20

Average of 10.374 to 10.380 min.: VL043016.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.90	63	133.85	49	142.00	104	148.75	246
123.70	186	134.95	458	143.00	3000	149.10	150
124.10	27	136.05	51	143.75	115	149.85	317
124.80	86	136.90	519	144.10	70	151.85	217
126.00	133	137.60	18	144.75	61	152.90	338
126.80	26	138.80	43	144.90	126	153.70	36
127.95	1014	139.10	84	145.10	91	153.95	131
128.95	580	139.60	25	145.70	120	154.95	663
129.80	458	140.05	132	145.95	202	156.00	51
130.00	698	140.90	2647	146.95	166	156.85	459
130.90	249	141.80	276	147.90	614	157.85	99

Average of 10.374 to 10.380 min.: VL043016.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.60	57	172.10	388				
158.90	282	173.00	610				
159.60	38	174.00	206144				
160.70	167	175.00	14877				
161.00	151	176.00	199189				
161.95	68	177.00	13044				
167.70	17	178.00	292				
169.80	43	204.90	28				
170.60	36	206.40	20				
171.10	105	206.80	37				
171.80	167	242.20	21				