


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100318\
 Data File : VL032581.D
 Acq On : 3 Oct 2018 15:07
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092418AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 01 06:49:26 2018
 Last Update : Mon Oct 01 06:49:26 2018

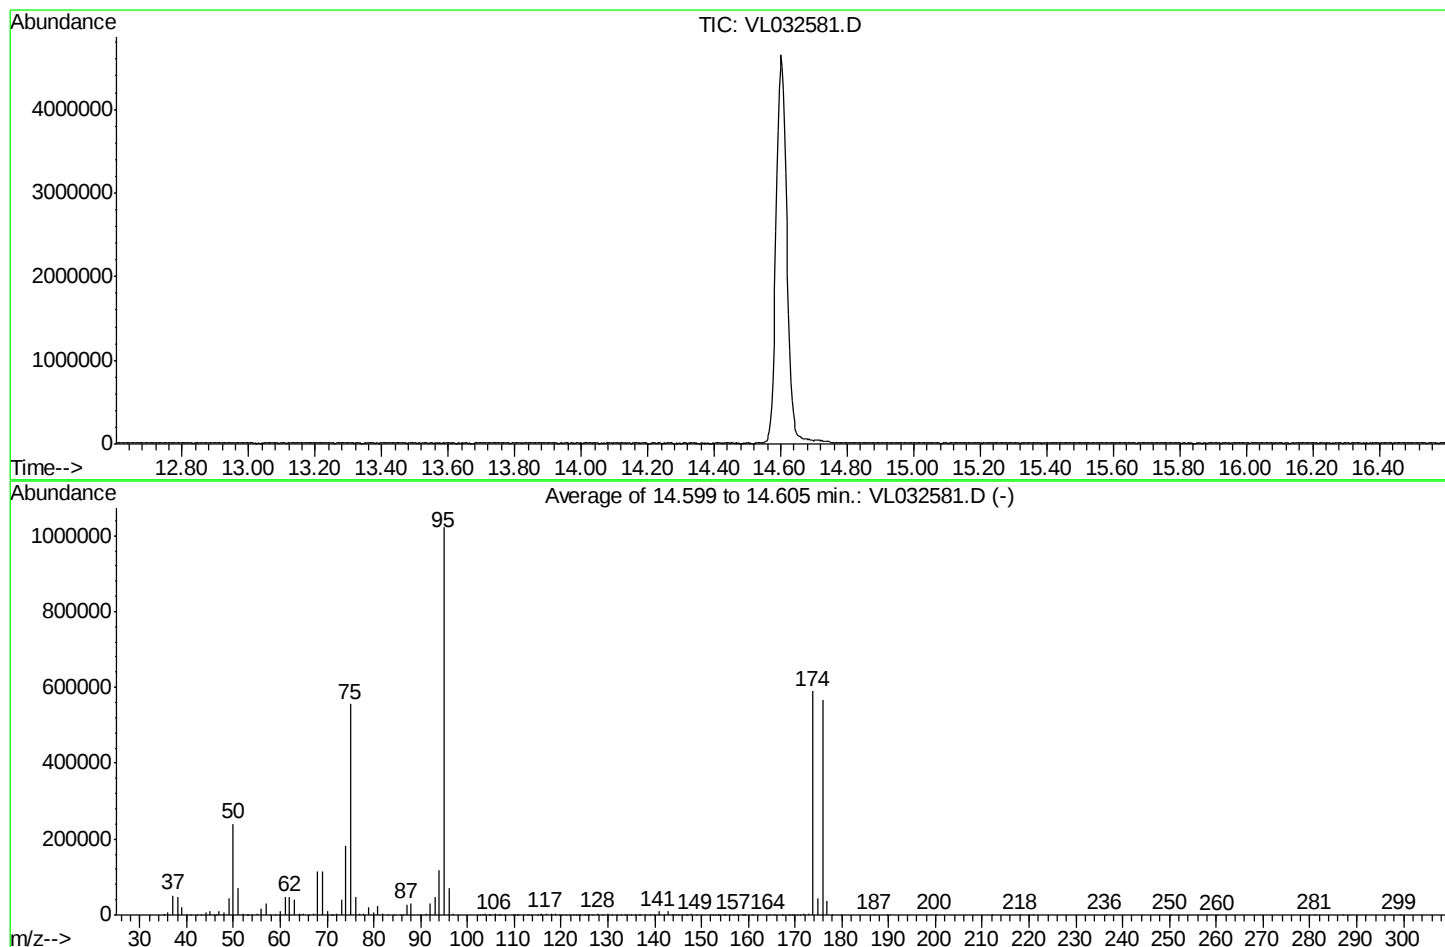

AutoFind: Scans 3627, 3628, 3629; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	239723	PASS
75	95	30	66	54.5	556544	PASS
95	95	100	100	100.0	1021909	PASS
96	95	5	9	6.9	70018	PASS
173	174	0.00	2	0.9	5153	PASS
174	95	50	120	57.7	589932	PASS
175	174	4	9	7.2	42400	PASS
176	174	93	101	96.2	567594	PASS
177	176	5	9	6.4	36120	PASS