


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100421\
 Data File : VL037757.D
 Acq On : 4 Oct 2021 9:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

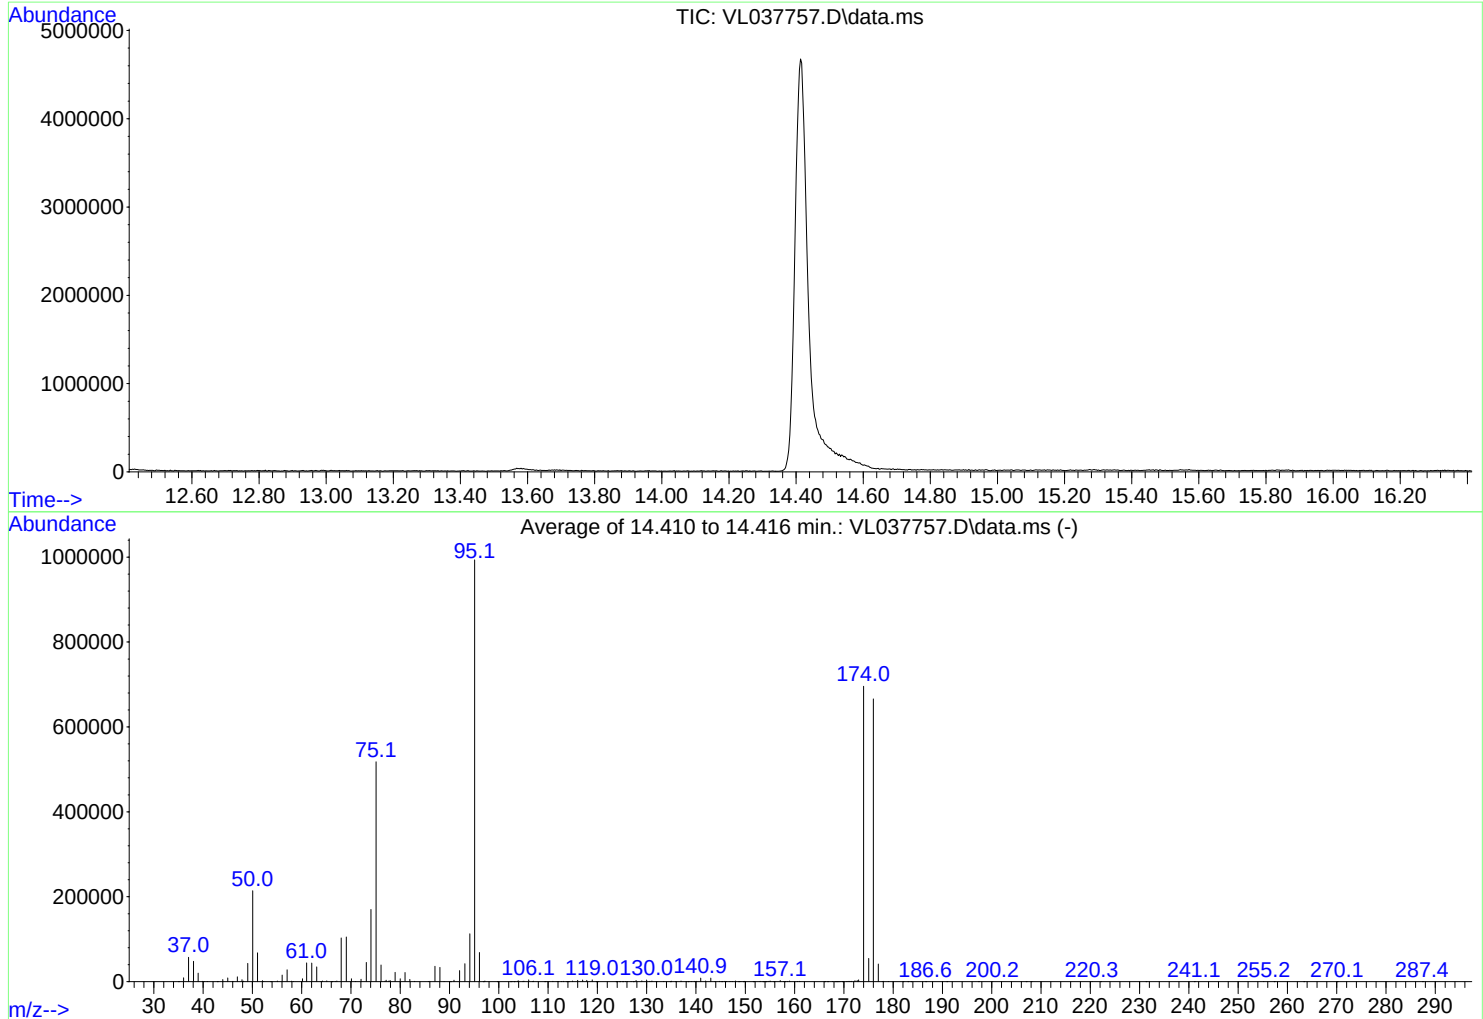

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.6	214293	PASS
75	95	30	66	52.1	517781	PASS
95	95	100	100	100.0	993600	PASS
96	95	5	9	6.9	68485	PASS
173	174	0.00	2	0.6	4079	PASS
174	95	50	120	70.0	695915	PASS
175	174	4	9	7.9	54872	PASS
176	174	93	101	95.7	666197	PASS
177	176	5	9	6.2	41384	PASS

Average of 14.410 to 14.416 min.: VL037757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.00	198	46.05	836	56.05	15504	66.10	170
36.05	9127	46.95	11427	57.05	27960	66.30	25
37.05	57453	47.90	4458	57.95	1111	66.80	50
38.05	48045	48.20	1278	58.30	273	67.15	150
39.00	20036	49.05	42941	60.15	6680	68.00	102973
39.90	716	50.05	214293	61.00	43968	69.05	105219
40.20	485	51.05	68011	62.05	43832	70.10	6751
40.85	235	52.05	2130	63.05	34797	70.95	523
42.90	214	52.30	534	63.90	560	72.05	5640
44.00	4963	53.70	78	64.20	1518	73.10	45317
45.00	8758	55.05	1673	65.10	1945	74.05	169856

Average of 14.410 to 14.416 min.: VL037757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	517781	85.70	429	96.05	68485	106.05	4350
76.10	39059	86.00	760	96.85	82	106.80	232
76.90	1339	87.05	36283	97.15	1403	107.05	1074
77.15	3306	88.05	33752	99.70	58	109.30	56
77.70	1449	88.90	311	102.40	81	109.80	266
77.95	2617	90.20	156	102.85	481	110.15	255
78.95	21784	90.90	3574	103.10	211	110.95	824
80.00	6876	92.05	26136	103.80	1160	111.85	273
80.95	21440	93.10	42344	104.00	1993	112.10	363
81.95	5203	94.10	112787	104.90	677	112.70	259
82.90	749	95.10	993600	105.10	1090	113.10	705

Average of 14.410 to 14.416 min.: VL037757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
113.75	211	124.05	312	131.05	1368	140.10	778
114.10	85	124.50	98	131.90	120	140.95	8432
114.95	1522	125.10	84	133.45	339	141.95	1521
116.00	2929	125.70	246	134.80	192	143.00	8407
117.00	3907	126.05	581	135.00	1133	143.85	358
117.85	2914	126.85	298	135.85	219	144.80	940
118.95	4086	127.30	201	136.95	1437	145.20	177
119.75	132	127.85	2674	138.05	331	145.85	766
120.00	94	129.00	1889	138.40	78	146.00	300
123.80	50	130.00	3873	139.05	442	146.20	488
123.90	95	130.65	731	139.75	664	146.90	388

Average of 14.410 to 14.416 min.: VL037757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.35	531	154.20	100	161.05	959	170.85	720
148.05	1463	154.80	830	166.10	79	171.20	633
148.65	220	155.05	1664	166.70	195	171.50	712
149.10	301	155.80	68	167.70	239	172.25	2429
149.60	109	155.95	268	168.30	88	172.70	2508
149.90	880	157.10	2570	168.60	176	173.00	4079
151.60	187	157.80	313	168.90	164	174.00	695915
151.90	518	158.00	131	169.40	418	175.05	54872
153.00	923	158.60	273	169.70	74	176.00	666197
153.60	112	159.00	1431	169.90	362	177.00	41384
153.90	203	160.60	307	170.60	266	177.80	525

Average of 14.410 to 14.416 min.: VL037757.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
178.05	742	220.35	294				
179.05	265	222.10	57				
182.00	152	231.30	55				
183.00	124	241.10	71				
183.60	63	255.20	227				
186.60	90	257.30	182				
190.90	66	263.30	59				

197.30	62	270.10	113
200.20	229	287.40	131
207.00	174		
208.00	108		

Instrument :
MSVOA_L
ClientSampleId :
BFB