


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100625\
Data File : VL043043.D
Acq On : 06 Oct 2025 07:57
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Oct 03 08:23:34 2025

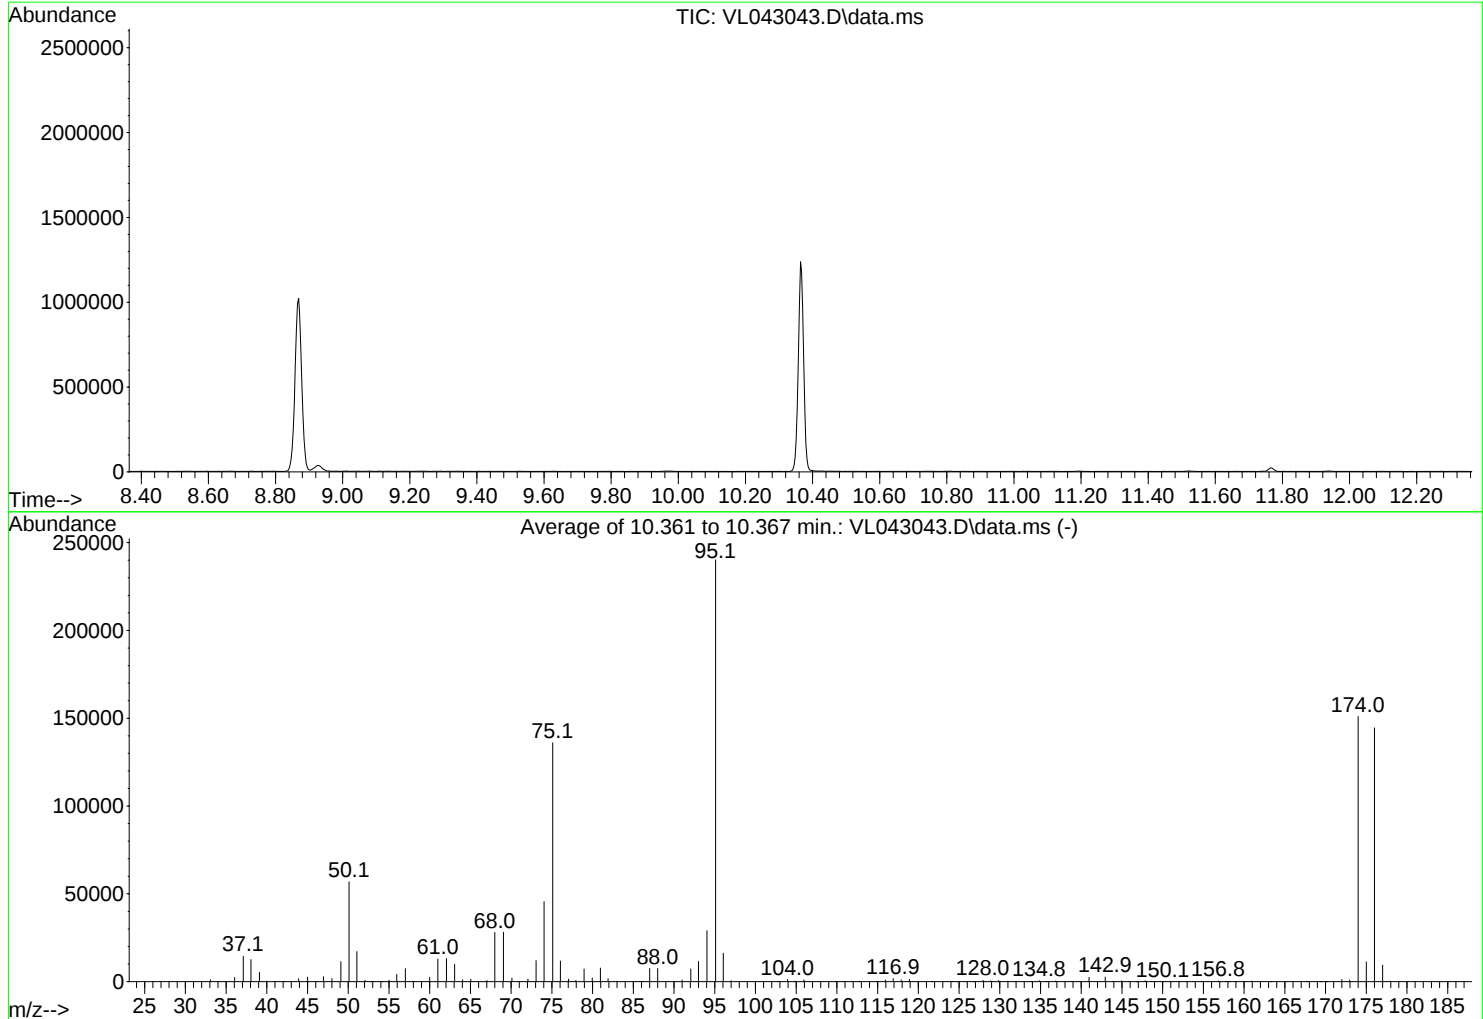

AutoFind: Scans 3174, 3175, 3176; Background Corrected with Scan 3159

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.7	56904	PASS
75	95	30	66	56.6	136077	PASS
95	95	100	100	100.0	240213	PASS
96	95	5	9	6.7	16210	PASS
173	174	0.00	2	0.6	956	PASS
174	95	50	120	62.9	150976	PASS
175	174	4	9	7.4	11194	PASS
176	174	93	101	95.7	144528	PASS
177	176	5	9	6.5	9360	PASS

Average of 10.361 to 10.367 min.: VL043043.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1003	43.90	1683	53.10	125	63.05	989
33.95	96	45.00	2533	53.90	62	64.05	112
35.00	24	46.00	168	54.10	35	65.05	133
36.05	2370	46.20	107	55.00	790	65.90	19
37.10	14494	46.95	2792	55.95	4089	66.90	225
38.05	12606	48.00	1765	57.00	7414	67.05	595
39.10	5293	49.10	11375	57.90	176	68.00	28048
39.95	349	50.10	56904	58.10	65	69.05	28187
40.90	23	51.05	17136	60.00	2391	70.10	2028
42.10	54	52.05	753	61.00	12894	72.05	1483
43.00	165	52.80	29	62.05	13089	73.05	11996

Average of 10.361 to 10.367 min.: VL043043.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.05	45589	86.10	92	103.95	1188	114.85	232
75.10	136077	87.00	7482	104.85	352	115.95	937
76.05	11795	88.00	7486	105.95	973	116.90	1707
77.05	1418	91.00	927	106.80	216	117.90	1028
77.95	762	92.05	7245	107.90	77	118.90	1301
78.95	7185	93.00	11489	109.80	212	121.70	20
79.95	2120	94.05	29013	110.70	108	123.70	135
80.95	7772	95.10	240213	111.00	143	124.10	23
81.90	1728	96.05	16210	111.80	61	124.75	70
82.95	261	97.00	555	112.05	131	125.90	63
85.80	193	102.80	110	112.75	243	126.80	41

Average of 10.361 to 10.367 min.: VL043043.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.95	763	139.90	80	148.70	140	156.85	392
128.90	485	140.95	2500	149.05	106	157.70	41
129.85	615	141.95	181	149.70	76	158.10	27
130.95	311	142.95	2695	150.05	169	158.85	91
131.90	42	143.85	159	151.00	20	159.10	78
133.90	47	144.95	501	151.90	41	160.95	329
134.85	596	145.80	120	153.00	206	163.30	20
135.70	50	146.05	207	153.70	67	167.70	26
136.85	407	146.80	24	154.00	60	169.40	29
138.80	89	146.95	149	154.80	297	170.10	33
139.70	134	147.85	593	155.00	190	172.00	1170

Average of 10.361 to 10.367 min.: VL043043.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.95	956						
174.00	150976						
175.00	11194						
176.00	144528						
177.00	9360						
177.95	363						

Instrument :

MSVOA_L

ClientSampleId :

BFB