

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100721\
 Data File : VL037818.D
 Acq On : 8 Oct 2021 5:35
 Operator : SY/AP
 Sample : M4079-03
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0P13

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.870	8	26	64	rBV	9119163	33917312	100.00%	24.850%
2	3.198	120	128	149	rBV	347960	631118	1.86%	0.462%
3	3.841	318	328	348	rBV	627500	1374251	4.05%	1.007%
4	4.337	472	482	502	rVB2	505611	953559	2.81%	0.699%
5	5.658	880	893	911	rBV3	2241227	5156820	15.20%	3.778%
6	7.163	1344	1361	1387	rBV2	4008457	8898645	26.24%	6.520%
7	7.465	1442	1455	1474	rBV4	145932	367458	1.08%	0.269%
8	10.417	2359	2373	2383	rBV6	228822	542717	1.60%	0.398%
9	11.211	2598	2620	2641	rBV	4887938	11539151	34.02%	8.454%
10	11.680	2752	2766	2786	rVB2	259820	692064	2.04%	0.507%
11	12.073	2864	2888	2908	rBV	4135396	10188349	30.04%	7.464%
12	12.333	2957	2969	2983	rVB4	192567	451093	1.33%	0.330%
13	13.545	3330	3346	3361	rBV10	150675	421811	1.24%	0.309%
14	14.400	3593	3612	3652	rBV2	3980276	11097952	32.72%	8.131%
15	15.298	3881	3891	3908	rVB2	163711	420813	1.24%	0.308%
16	16.085	4118	4136	4139	rBV8	234673	561555	1.66%	0.411%
17	16.111	4139	4144	4157	rVB5	226855	426787	1.26%	0.313%
18	16.609	4288	4299	4309	rBV8	182266	398199	1.17%	0.292%
19	16.963	4386	4409	4427	rBV2	1407248	4169187	12.29%	3.055%
20	17.519	4565	4582	4609	rBV4	658904	2176417	6.42%	1.595%
21	17.670	4618	4629	4644	rVB3	177183	424993	1.25%	0.311%
22	17.921	4691	4707	4721	rBV4	774470	2037278	6.01%	1.493%
23	18.156	4762	4780	4783	rBV	321328	533895	1.57%	0.391%
24	18.342	4817	4838	4856	rBV2	2760506	7645036	22.54%	5.601%
25	18.796	4961	4979	4988	rVV6	276818	806732	2.38%	0.591%
26	18.889	4991	5008	5022	rVV3	2026121	5971447	17.61%	4.375%
27	18.944	5022	5025	5040	rVV4	656486	1201871	3.54%	0.881%
28	19.043	5040	5056	5072	rVV3	1189878	2912462	8.59%	2.134%
29	19.194	5083	5103	5121	rVB8	399167	1202585	3.55%	0.881%
30	19.442	5158	5180	5193	rBV4	1254825	3948529	11.64%	2.893%
31	19.494	5193	5196	5215	rVB4	475801	876954	2.59%	0.643%
32	19.728	5249	5269	5280	rBV8	252627	802623	2.37%	0.588%
33	19.799	5283	5291	5310	rVB6	311226	763414	2.25%	0.559%
34	19.956	5324	5340	5343	rBV7	212132	414891	1.22%	0.304%

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100721\
Data File : VL037818.D
Acq On : 8 Oct 2021 5:35
Operator : SY/AP
Sample : M4079-03
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P13

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 3 Min Area: 3 % of largest Peak
Start Thrs: 0.001 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

35	20.027	5352	5362	5382	rVB6	324781	993056	2.93%	0.728%
36	20.522	5504	5516	5530	rBV6	198614	605235	1.78%	0.443%
37	21.001	5662	5665	5680	rVB6	219747	353519	1.04%	0.259%
38	21.461	5789	5808	5824	rBV2	519909	1569606	4.63%	1.150%
39	21.989	5953	5972	5985	rBV2	231099	763953	2.25%	0.560%
40	22.178	6013	6031	6056	rBV2	357663	1379563	4.07%	1.011%
41	22.696	6186	6192	6207	rVB2	195170	433207	1.28%	0.317%
42	22.908	6246	6258	6266	rBV2	260375	637918	1.88%	0.467%
43	23.169	6320	6339	6340	rBV2	205632	449278	1.32%	0.329%
44	23.220	6344	6355	6372	rVB2	354631	1113328	3.28%	0.816%
45	23.339	6376	6392	6393	rBV2	214449	438057	1.29%	0.321%
46	24.374	6699	6714	6718	rBV10	288056	730450	2.15%	0.535%
47	24.590	6769	6781	6788	rBV5	498534	1055373	3.11%	0.773%
48	24.808	6835	6849	6856	rVB6	365054	793273	2.34%	0.581%
49	24.982	6893	6903	6904	rBV10	290902	339882	1.00%	0.249%
50	26.403	7329	7345	7359	rVB10	383843	907150	2.67%	0.665%


Sum of corrected areas: 136490816

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100721\
Data File : VL037818.D
Acq On : 8 Oct 2021 5:35
Operator : SY/AP
Sample : M4079-03
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

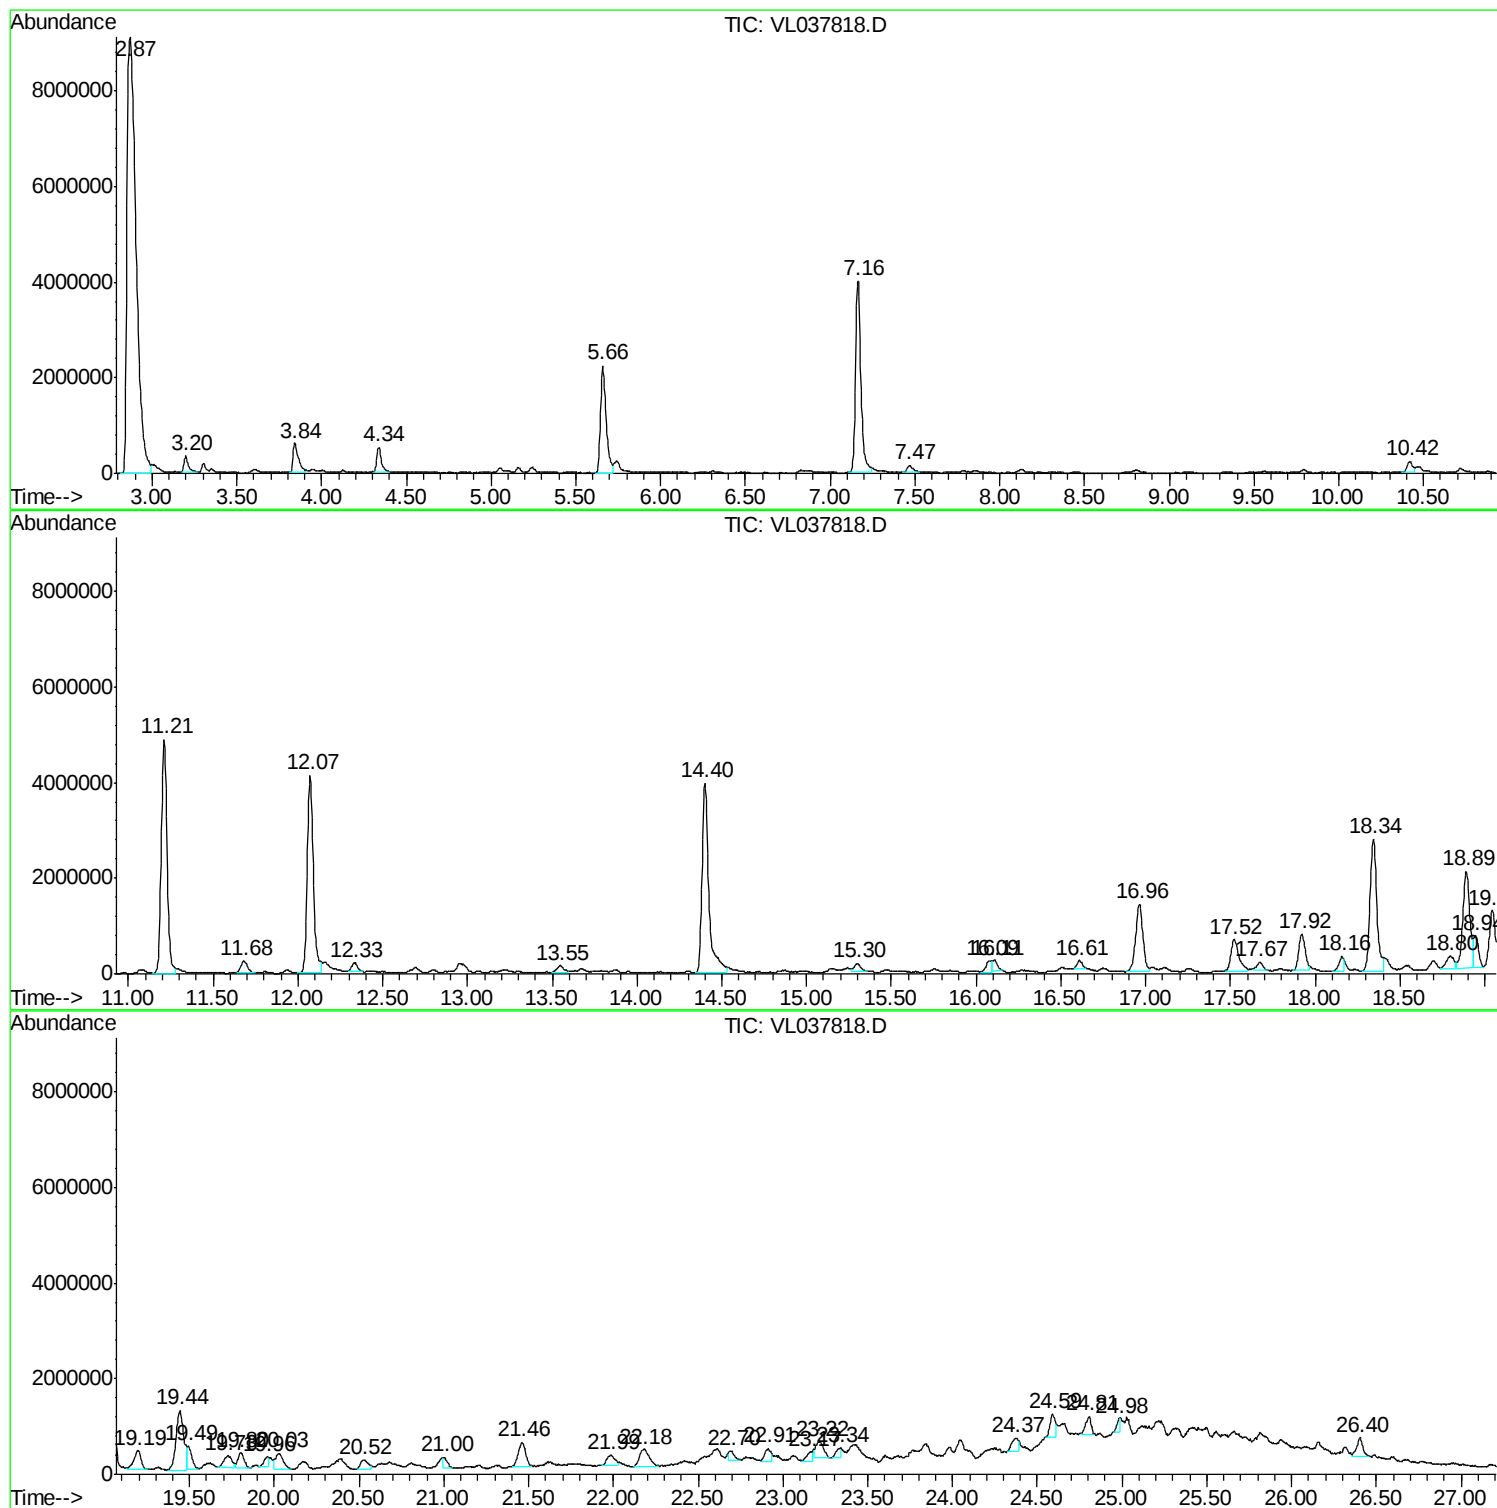

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100721\
Data File : VL037818.D
Acq On : 8 Oct 2021 5:35
Operator : SY/AP
Sample : M4079-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100721\
Data File : VL037818.D
Acq On : 8 Oct 2021 5:35
Operator : SY/AP
Sample : M4079-03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc