

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100721\
 Data File : VL037823.D
 Acq On : 8 Oct 2021 9:05
 Operator : SY/AP
 Sample : M4012-01
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0P23

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.867	11	25	63	rBV	7357547	21064545	32.33%	7.324%
2	3.018	63	72	97	rVB4	1082915	2138561	3.28%	0.744%
3	3.195	117	127	153	rBV2	7663901	14043301	21.55%	4.883%
4	3.346	166	174	189	rVB2	609597	928064	1.42%	0.323%
5	3.632	238	263	307	rBV	14709387	65151249	100.00%	22.652%
6	3.835	316	326	356	rBV	12213363	30669303	47.07%	10.663%
7	3.989	356	374	406	rVV2	5996593	18813517	28.88%	6.541%
8	4.121	406	415	424	rVV2	668755	1103426	1.69%	0.384%
9	4.179	424	433	448	rVB5	434631	853685	1.31%	0.297%
10	4.333	462	481	508	rBV	3669338	7552490	11.59%	2.626%
11	5.665	879	895	913	rBV4	3663210	9316154	14.30%	3.239%
12	5.735	913	917	936	rVB4	315848	678844	1.04%	0.236%
13	6.298	1079	1092	1117	rBV7	313204	895671	1.37%	0.311%
14	6.809	1236	1251	1266	rBV3	472264	1481431	2.27%	0.515%
15	7.160	1330	1360	1378	rBV3	4267236	9690524	14.87%	3.369%
16	8.108	1642	1655	1680	rBV5	278343	750532	1.15%	0.261%
17	8.803	1858	1871	1889	rVB4	809870	1844148	2.83%	0.641%
18	9.790	2160	2178	2203	rBV	1406544	3109403	4.77%	1.081%
19	10.404	2356	2369	2381	rBV4	771994	1771958	2.72%	0.616%
20	10.947	2526	2538	2552	rBV4	332004	729732	1.12%	0.254%
21	11.069	2560	2576	2596	rBV9	440053	1224227	1.88%	0.426%
22	12.069	2869	2887	2907	rVV2	4633098	11428110	17.54%	3.973%
23	12.169	2907	2918	2942	rVB7	484964	1510806	2.32%	0.525%
24	12.330	2956	2968	2982	rVB6	314620	717198	1.10%	0.249%
25	12.693	3060	3081	3096	rBV2	472272	1189207	1.83%	0.413%
26	12.796	3099	3113	3125	rBV5	395111	902591	1.39%	0.314%
27	12.947	3147	3160	3183	rVB2	851220	2608482	4.00%	0.907%
28	13.076	3183	3200	3215	rVB5	385319	1105911	1.70%	0.385%
29	13.384	3282	3296	3316	rVB3	1536640	3586611	5.51%	1.247%
30	13.526	3324	3340	3342	rBV6	484352	935702	1.44%	0.325%
31	13.536	3342	3343	3366	rVB6	471044	745215	1.14%	0.259%
32	13.671	3366	3385	3398	rBV3	470684	1257627	1.93%	0.437%
33	13.864	3437	3445	3459	rVB3	515553	1163310	1.79%	0.404%
34	14.127	3512	3527	3547	rVB2	1995741	4499853	6.91%	1.565%

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100721\
 Data File : VL037823.D
 Acq On : 8 Oct 2021 9:05
 Operator : SY/AP
 Sample : M4012-01
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0P23

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 3 Min Area: 3 % of largest Peak
 Start Thrs: 0.001 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

35	14.397	3592	3611	3627	rBV2	4830934	11642515	17.87%	4.048%
36	14.468	3631	3633	3651	rVB6	504200	920808	1.41%	0.320%
37	14.863	3738	3756	3767	rBV5	314479	802090	1.23%	0.279%
38	15.153	3826	3846	3854	rBV5	531795	1428251	2.19%	0.497%
39	15.214	3854	3865	3879	rVV7	629021	1857141	2.85%	0.646%
40	15.294	3879	3890	3908	rVB4	715633	1848650	2.84%	0.643%
41	16.005	4102	4111	4121	rVV4	316263	741301	1.14%	0.258%
42	16.079	4121	4134	4154	rVB8	525203	1750749	2.69%	0.609%
43	16.545	4262	4279	4290	rVV7	364603	1157798	1.78%	0.403%
44	16.748	4328	4342	4358	rBV8	491662	1297190	1.99%	0.451%
45	16.957	4387	4407	4435	rBV2	2768571	8263031	12.68%	2.873%
46	17.092	4435	4449	4468	rVV3	1886628	4516157	6.93%	1.570%
47	17.796	4651	4668	4683	rBV5	450716	1114833	1.71%	0.388%
48	17.928	4692	4709	4726	rBV5	1502485	4277967	6.57%	1.487%
49	18.153	4762	4779	4791	rBV5	373972	1042410	1.60%	0.362%
50	18.339	4825	4837	4862	rVB6	458784	1448865	2.22%	0.504%
51	18.931	5012	5021	5038	rVB8	391660	1095061	1.68%	0.381%
52	19.490	5185	5195	5212	rVB4	401308	899702	1.38%	0.313%
53	19.886	5304	5318	5337	rBV3	958739	2386015	3.66%	0.830%
54	21.458	5781	5807	5830	rBV	2650428	9267517	14.22%	3.222%
55	22.442	6098	6113	6129	rVB7	369439	1077363	1.65%	0.375%
56	22.773	6199	6216	6232	rBV4	664158	1747997	2.68%	0.608%
57	23.207	6333	6351	6368	rVB9	221433	672063	1.03%	0.234%
58	25.053	6914	6925	6936	rVB3	478266	900016	1.38%	0.313%


Sum of corrected areas: 287616878

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL100721\
Data File : VL037823.D
Acq On : 8 Oct 2021 9:05
Operator : SY/AP
Sample : M4012-01
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P23

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

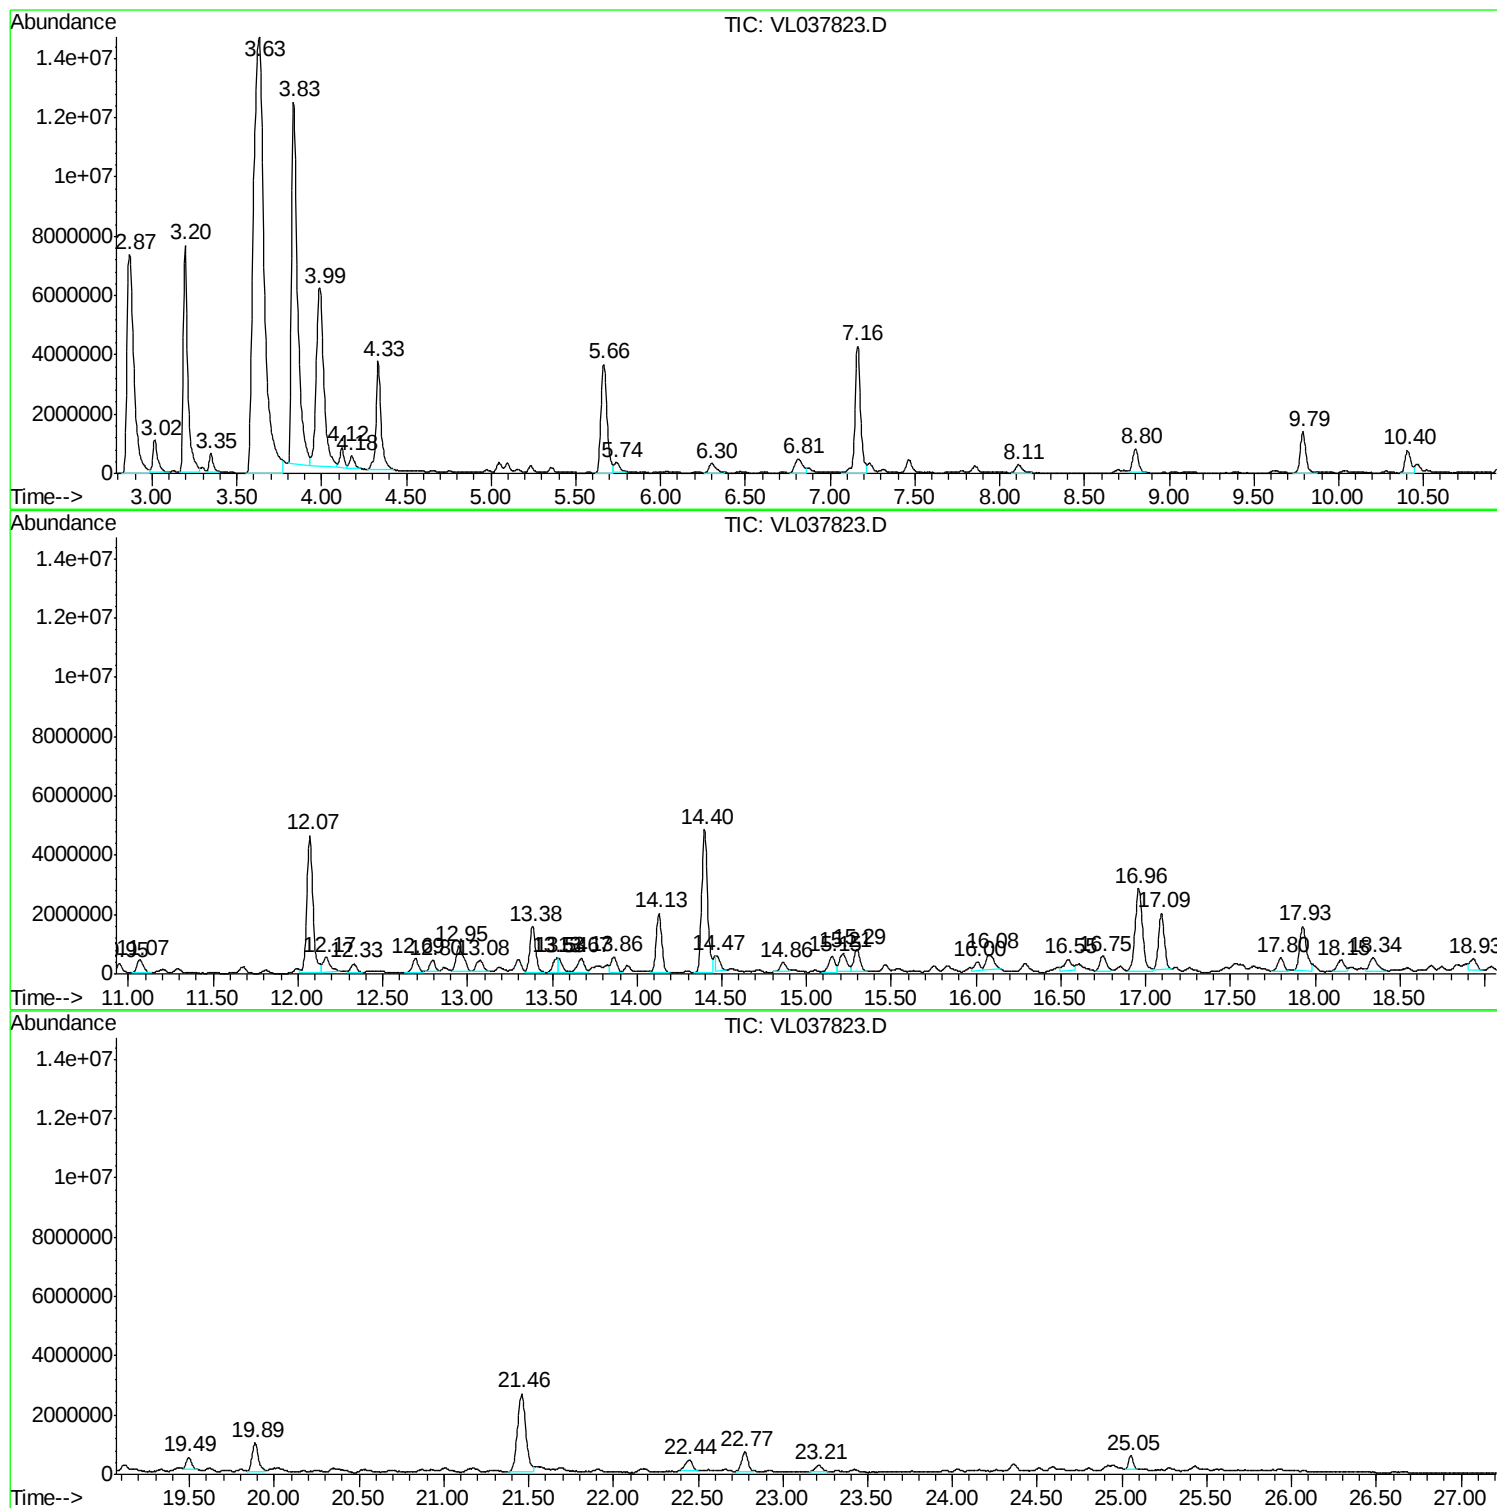

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100721\
Data File : VL037823.D
Acq On : 8 Oct 2021 9:05
Operator : SY/AP
Sample : M4012-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P23

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100721\
Data File : VL037823.D
Acq On : 8 Oct 2021 9:05
Operator : SY/AP
Sample : M4012-01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
C0P23

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc