


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL100721\
 Data File : VL037795.D
 Acq On : 7 Oct 2021 13:09
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

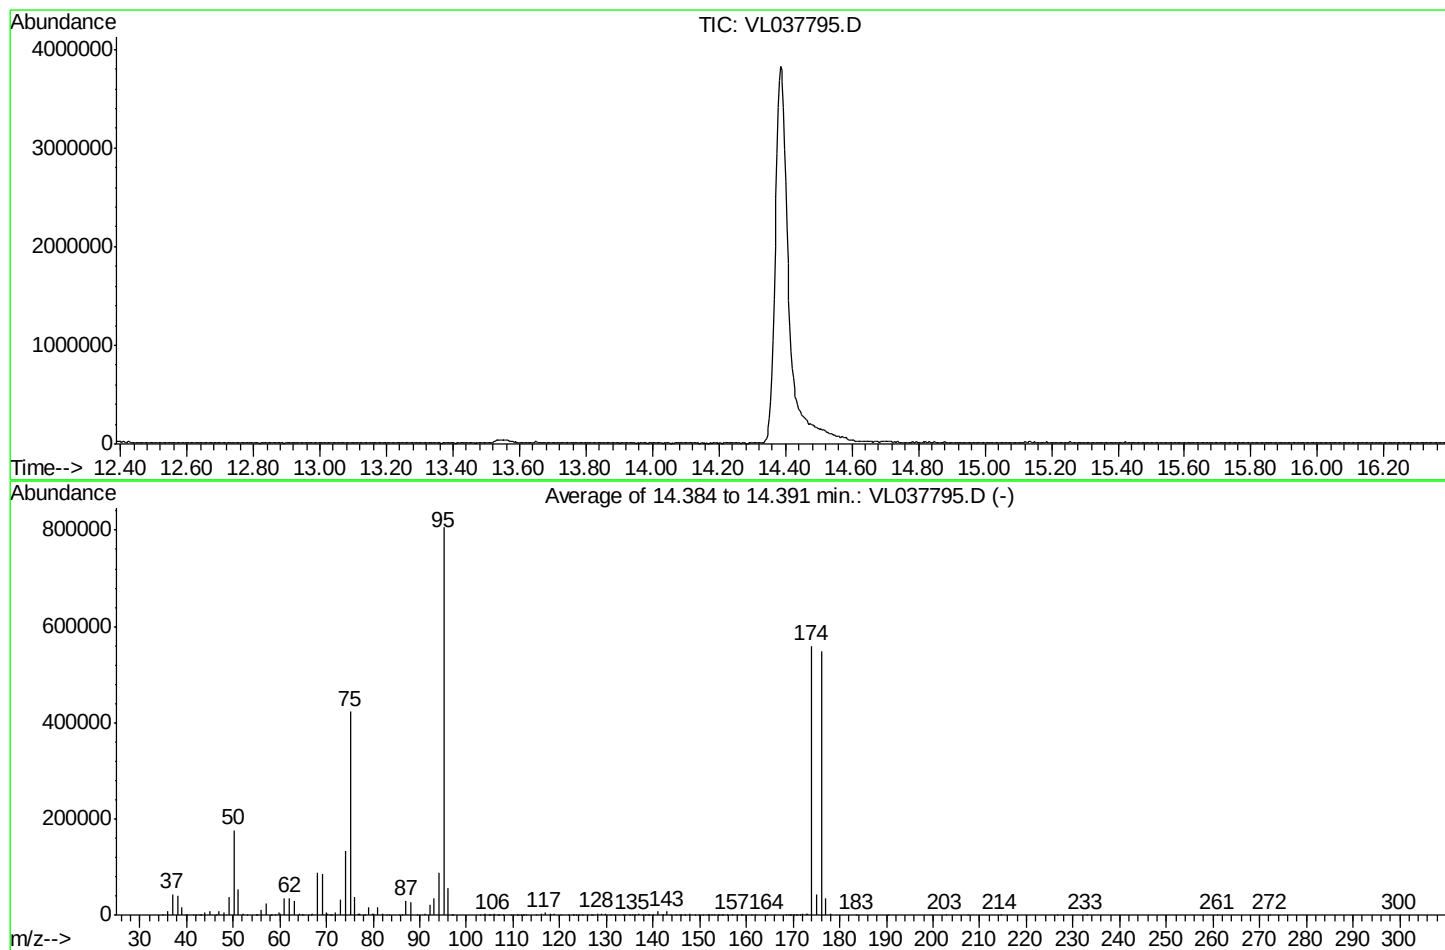

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.9	176661	PASS
75	95	30	66	52.5	422954	PASS
95	95	100	100	100.0	806080	PASS
96	95	5	9	6.9	55656	PASS
173	174	0.00	2	0.5	2810	PASS
174	95	50	120	69.5	560128	PASS
175	174	4	9	7.5	42042	PASS
176	174	93	101	97.7	547477	PASS
177	176	5	9	6.3	34461	PASS