

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100825\
 Data File : VL043058.D
 Acq On : 08 Oct 2025 11:43
 Operator : SY/MD
 Sample : QC100725 CAN 10420
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC100725 CAN 10420

Quant Time: Oct 09 01:15:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Oct 03 08:23:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.794	49	180369	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	3.965	114	479249	10.000	ppbv	0.03
55) Chlorobenzene-d5	8.888	117	385348	10.000	ppbv	0.03

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.383	95	263585	9.495	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100825\
Data File : VL043058.D
Acq On : 08 Oct 2025 11:43
Operator : SY/MD
Sample : QC100725 CAN 10420
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC100725 CAN 10420

Quant Time: Oct 09 01:15:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Oct 03 08:23:34 2025
Response via : Initial Calibration




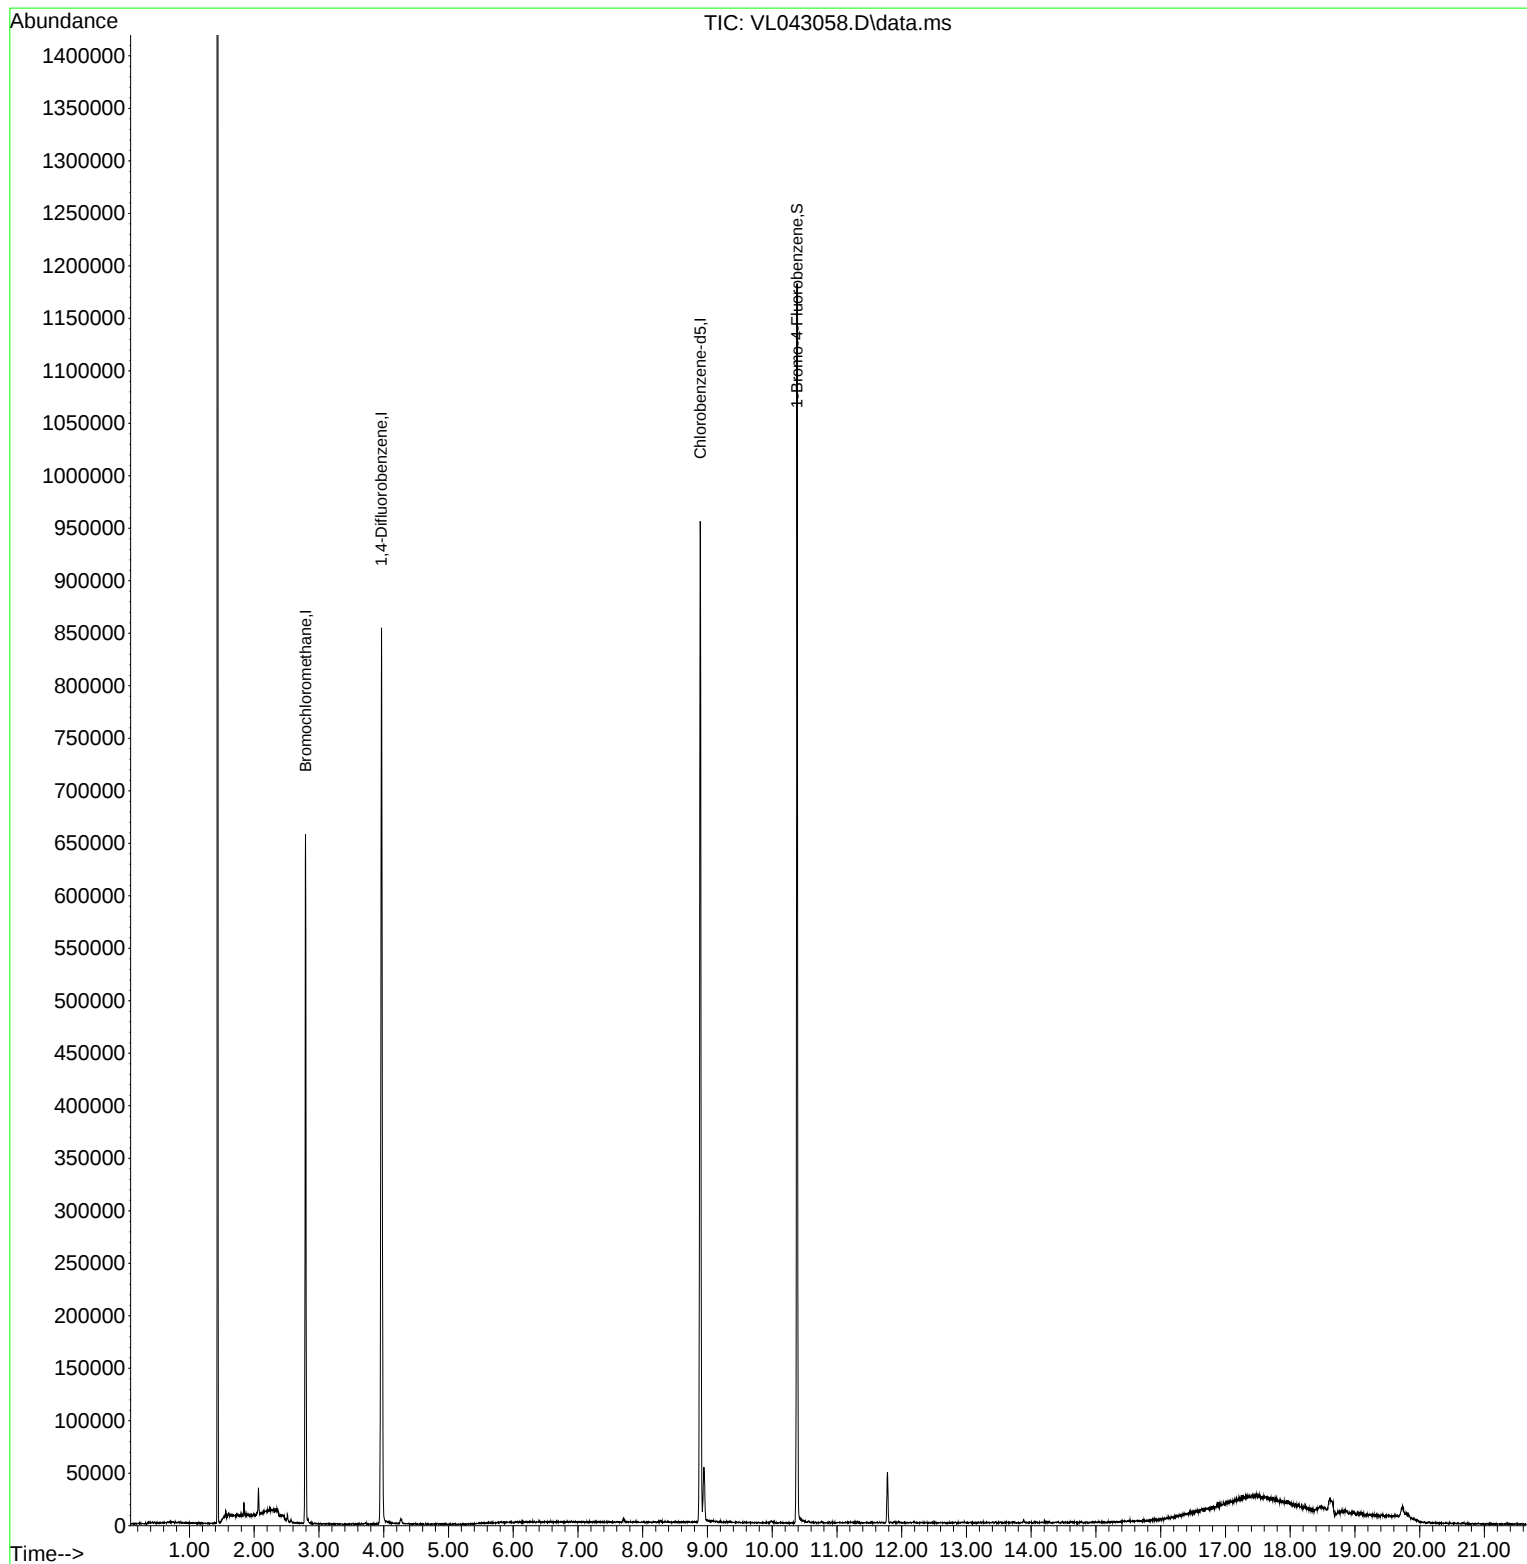


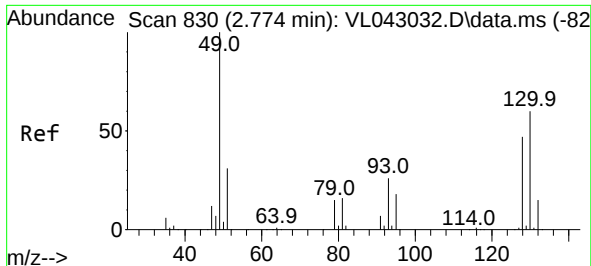

#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 2.794 min Scan# 81
 Delta R.T. 0.020 min
 Lab File: VL043058.D
 Acq: 08 Oct 2025 11:43




Instrument :
 MSVOA_L
 ClientSampleId :
 QC100725 CAN 10420


Tgt Ion: 49 Resp: 180369
 Ion Ratio Lower Upper
 49 100
 128 47.5 24.1 72.2
 130 60.0 31.4 94.3

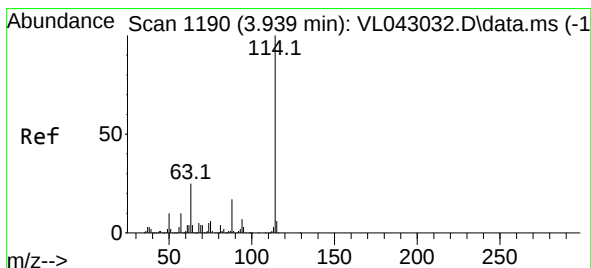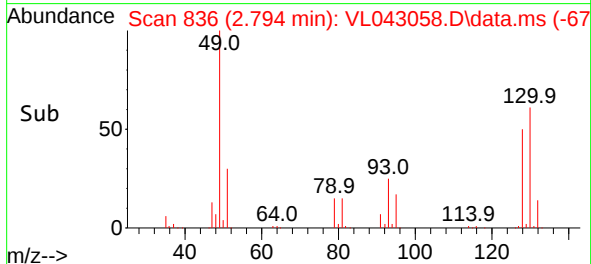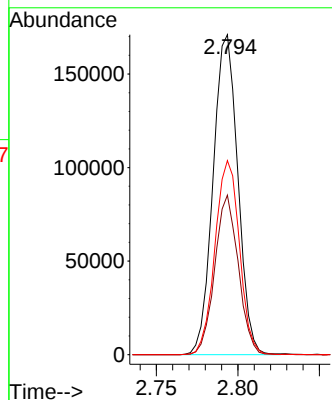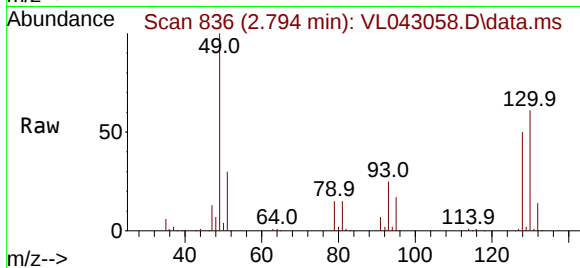

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 3.965 min Scan# 1198
 Delta R.T. 0.026 min
 Lab File: VL043058.D
 Acq: 08 Oct 2025 11:43

Tgt Ion:114 Resp: 479249
 Ion Ratio Lower Upper
 114 100
 63 25.1 19.4 29.2
 88 17.9 13.9 20.9


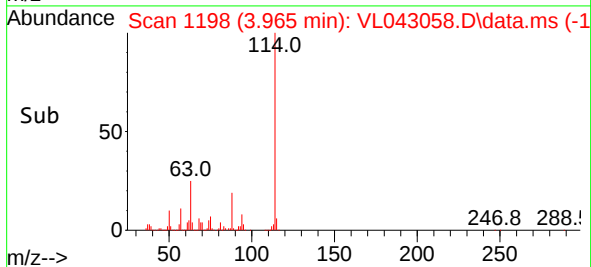
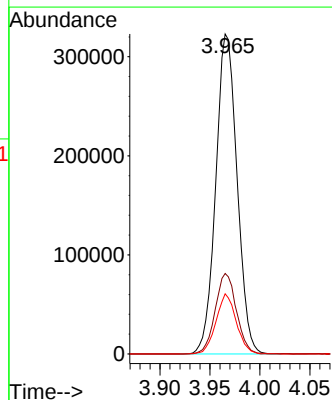
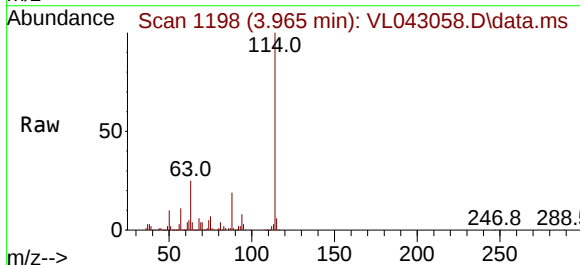


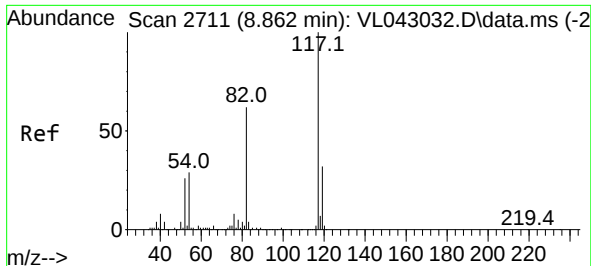

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.888 min Scan# 21
Delta R.T. 0.026 min
Lab File: VL043058.D
Acq: 08 Oct 2025 11:43

Instrument :
MSVOA_L
ClientSampleId :
QC100725 CAN 10420

Tgt Ion:117 Resp: 385348
Ion Ratio Lower Upper
117 100
82 63.5 53.0 79.6
119 31.7 25.4 38.2

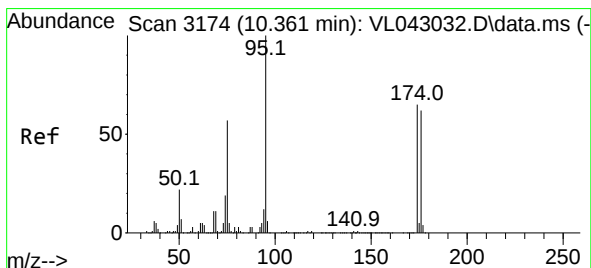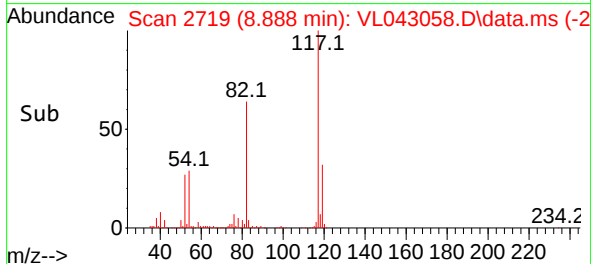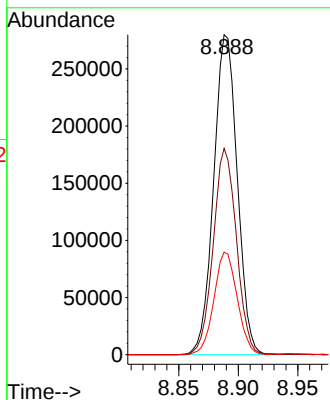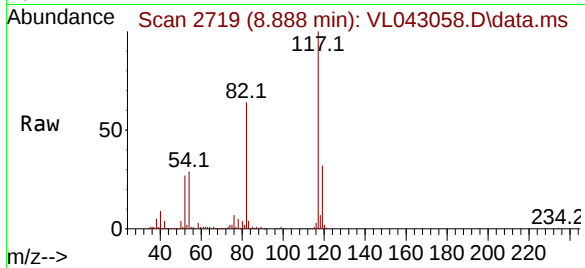

#68
1-Bromo-4-Fluorobenzene
Concen: 9.495 ppbv
RT: 10.383 min Scan# 3181
Delta R.T. 0.023 min
Lab File: VL043058.D
Acq: 08 Oct 2025 11:43

Tgt Ion: 95 Resp: 263585
Ion Ratio Lower Upper
95 100
174 65.4 52.3 78.5
175 4.7 3.8 5.8

