

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100925\
 Data File : VL043090.D
 Acq On : 09 Oct 2025 16:07
 Operator : SY/MD
 Sample : Q3320-08 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV4

Quant Time: Oct 09 22:17:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Oct 03 08:23:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	2.777	49	198803	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.942	114	523879	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.865	117	525878	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.364	95	427637	11.288	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	112.900%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.496	85	1606	0.048	ppbv	93
3) Chlorodifluoromethane	1.619	51	985	0.030	ppbv	92
9) Propene	1.483	41	2658	0.203	ppbv #	17
10) Heptane	4.959	43	9039	0.281	ppbv	100
11) Trichlorofluoromethane	1.871	101	3244	0.094	ppbv	95
13) Ethanol	1.719	45	3306	5.711	ppbv #	31
15) Acetone	1.829	43	512933	18.427	ppbv	98
16) 1,3-Butadiene	1.596	39	1019	0.089	ppbv #	81
17) tert-Butyl alcohol	2.039	59	1398	0.047	ppbv #	59
19) Isopropyl Alcohol	1.881	45	5339	0.400	ppbv #	1
20) Methylene Chloride	2.056	84	3855	0.317	ppbv	93
23) Vinyl Acetate	2.460	43	729	0.123	ppbv #	48
25) Ethyl Acetate	2.816	43	46640	0.668	ppbv #	76
26) Hexane	2.816	57	64733	2.410	ppbv #	33
27) Carbon Disulfide	2.140	76	3284	0.104	ppbv #	1
30) Cyclohexane	3.836	84	1599	0.072	ppbv #	49
34) 2-Butanone	2.554	43	14981	0.421	ppbv	96
36) Benzene	3.645	78	2146	0.043	ppbv	95
38) Trichloroethene	4.528	130	1672	0.080	ppbv #	77
39) 1,2-Dichloropropane	3.942	63	134036	7.225	ppbv #	22
41) Tetrahydrofuran	3.049	42	2343	0.128	ppbv #	78
51) 2-Hexanone	7.409	43	2707	0.088	ppbv #	29
52) Tetrachloroethene	8.215	164	1021	0.055	ppbv #	85
53) Toluene	6.910	91	21425	0.424	ppbv	99
58) Ethyl Benzene	9.341	91	8236	0.101	ppbv	93
59) m/p-Xylene	9.542	91	2540	0.037	ppbv #	30
60) o-Xylene	9.950	91	12540	0.183	ppbv	93
63) 1,1,2,2-Tetrachloroethane	9.934	83	4096	0.083	ppbv #	90
64) n-propylbenzene	10.976	120	888	0.033	ppbv #	1
66) Benzyl Chloride	11.623	91	186	0.052	ppbv #	65
71) 2-Chlorotoluene	10.979	91	3370	0.044	ppbv	92
73) 1,3,5-Trimethylbenzene	11.189	105	3600	0.051	ppbv #	71
74) 1,2,4-Trimethylbenzene	11.523	105	3947	0.050	ppbv #	57
79) Naphthalene	13.507	128	397	0.240	ppbv #	58
80) Naphthalene,2-methyl-	14.452	142	652	0.682	ppbv #	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100925\
Data File : VL043090.D
Acq On : 09 Oct 2025 16:07
Operator : SY/MD
Sample : Q3320-08 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV4

Quant Time: Oct 09 22:17:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Oct 03 08:23:34 2025
Response via : Initial Calibration




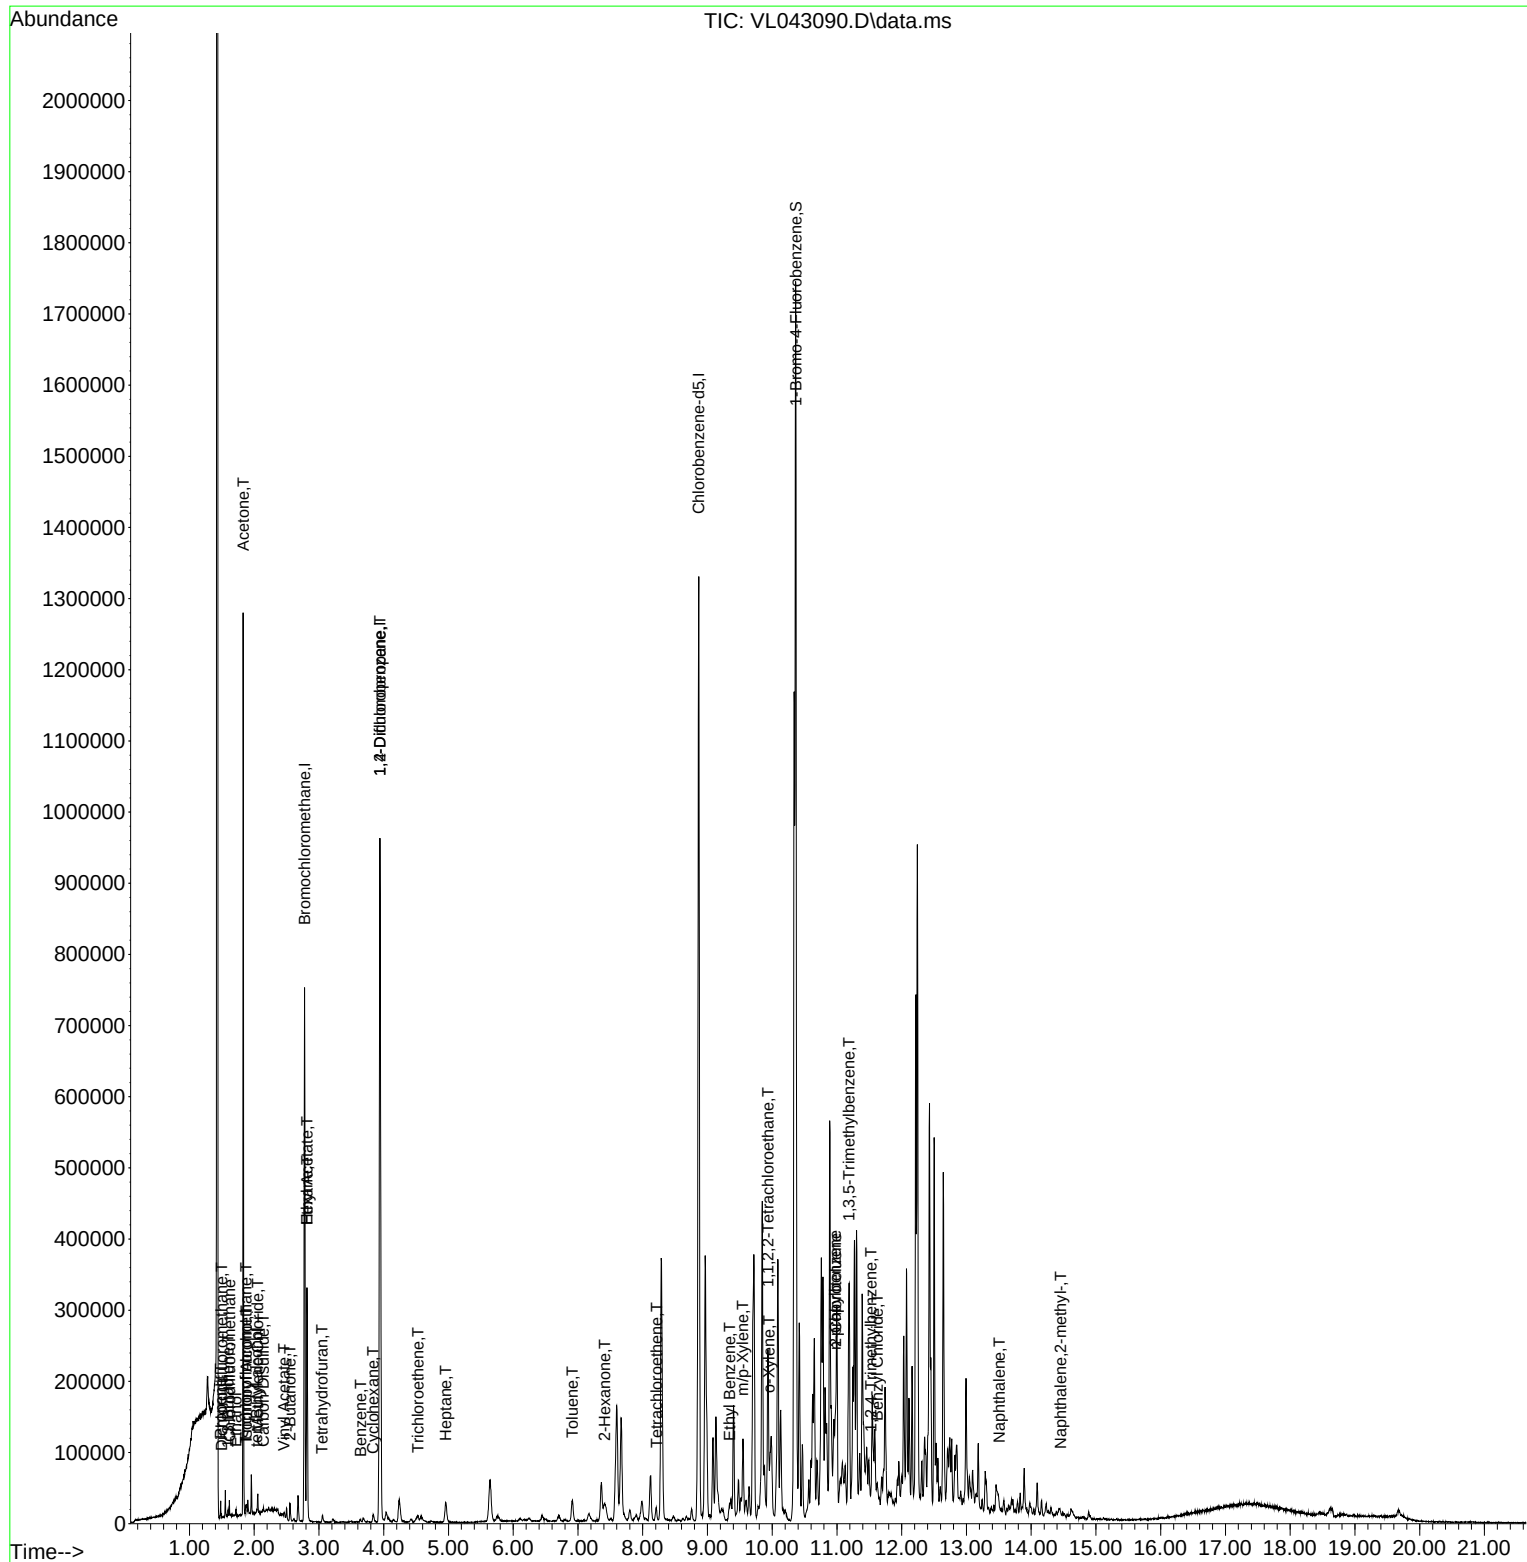




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.777 min Scan# 831
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 49 Resp: 198803
Ion Ratio Lower Upper
49 100
128 47.0 24.1 72.2
130 60.4 31.4 94.3



#2
Dichlorodifluoromethane
Concen: 0.048 ppbv
RT: 1.496 min Scan# 435
Delta R.T. 0.000 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 85 Resp: 1606
Ion Ratio Lower Upper
85 100
87 35.9 25.8 38.6


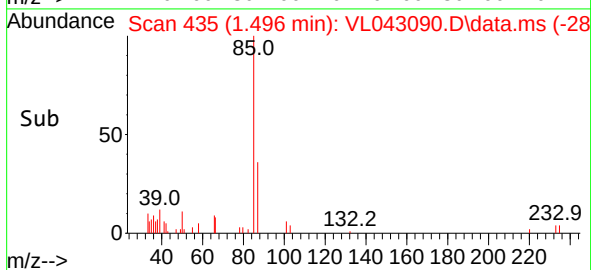






#3
Chlorodifluoromethane
Concen: 0.030 ppbv
RT: 1.619 min Scan# 41
Delta R.T. 0.146 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 51 Resp: 985
Ion Ratio Lower Upper
51 100
67 22.4 15.1 22.7

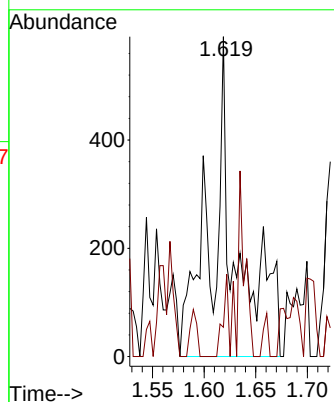

#9
Propene
Concen: 0.203 ppbv
RT: 1.483 min Scan# 431
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 41 Resp: 2658
Ion Ratio Lower Upper
41 100
42 0.0 53.3 79.9#


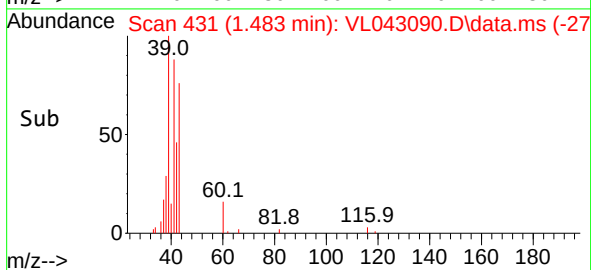
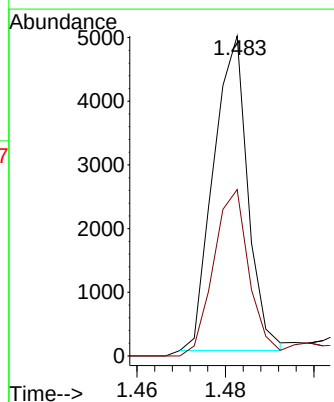





#10
Heptane
Concen: 0.281 ppbv
RT: 4.959 min Scan# 11
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 43 Resp: 9039
Ion Ratio Lower Upper
43 100
57 50.3 40.3 60.5



#11
Trichlorofluoromethane
Concen: 0.094 ppbv
RT: 1.871 min Scan# 551
Delta R.T. 0.000 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion:101 Resp: 3244
Ion Ratio Lower Upper
101 100
103 67.6 51.1 76.7









#13
 Ethanol
 Concen: 5.711 ppbv
 RT: 1.719 min Scan# 503
 Delta R.T. 0.003 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07




Instrument :
 MSVOA_L
 ClientSampleId :
 SV4


Tgt Ion: 45 Resp: 3306
 Ion Ratio Lower Upper
 45 100
 46 0.0 17.8 71.4#

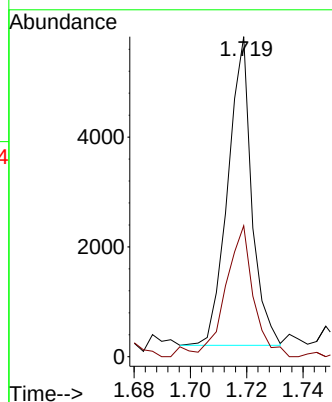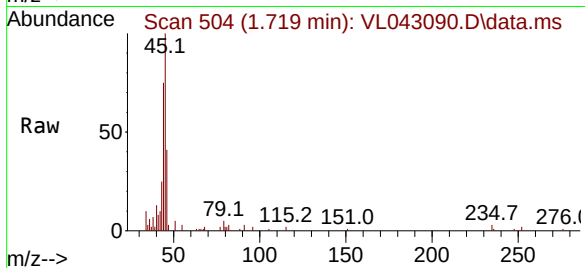

#15
 Acetone
 Concen: 18.427 ppbv
 RT: 1.829 min Scan# 538
 Delta R.T. 0.000 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07

Tgt Ion: 43 Resp: 512933
 Ion Ratio Lower Upper
 43 100
 58 29.0 22.2 33.4



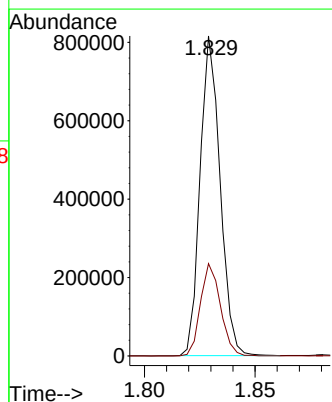
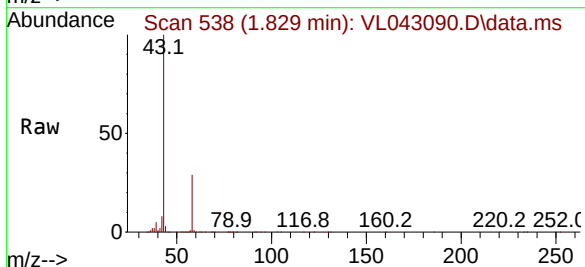




#16
1,3-Butadiene
Concen: 0.089 ppbv
RT: 1.596 min Scan# 466
Delta R.T. -0.010 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 39 Resp: 1019
Ion Ratio Lower Upper
39 100
54 60.5 61.4 92.2#

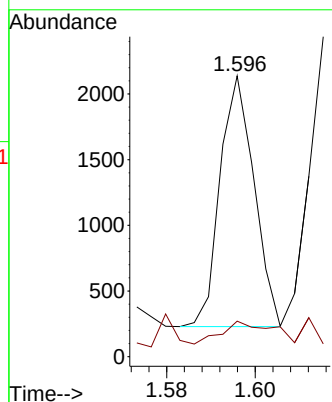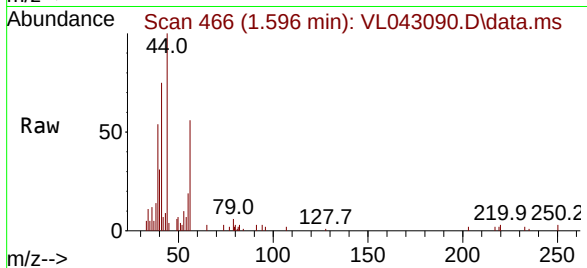

#17
tert-Butyl alcohol
Concen: 0.047 ppbv
RT: 2.039 min Scan# 603
Delta R.T. 0.007 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 59 Resp: 1398
Ion Ratio Lower Upper
59 100
57 26.2 8.5 12.7#



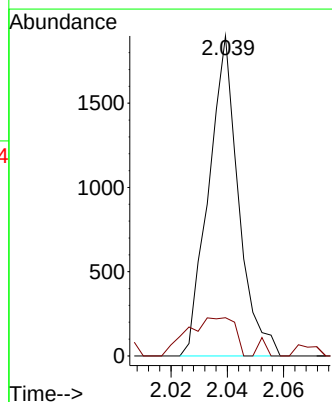
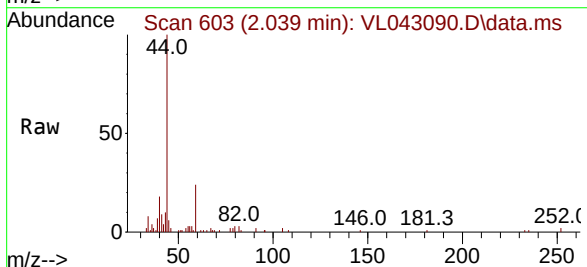




#19
Isopropyl Alcohol
Concen: 0.400 ppbv
RT: 1.881 min Scan# 51
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 45 Resp: 5339
Ion Ratio Lower Upper
45 100
58 2781.6 42.3 63.5#

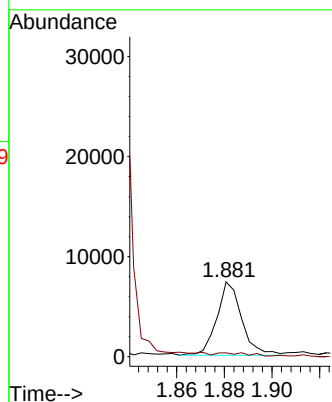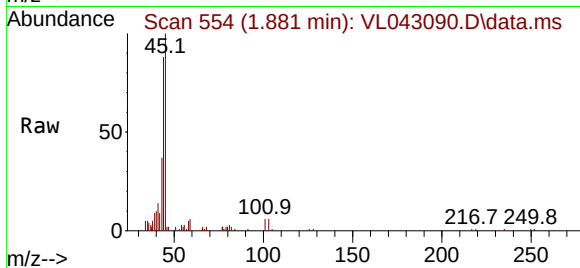

#20
Methylene Chloride
Concen: 0.317 ppbv
RT: 2.056 min Scan# 608
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 84 Resp: 3855
Ion Ratio Lower Upper
84 100
49 130.9 112.5 168.7
51 49.9 34.2 51.2
86 61.3 48.4 72.6

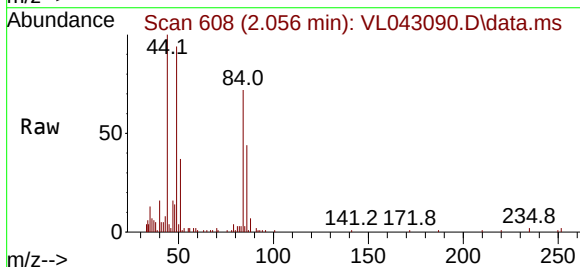







#23
 Vinyl Acetate
 Concen: 0.123 ppbv
 RT: 2.460 min Scan# 71
 Delta R.T. 0.010 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07

Instrument :
 MSVOA_1
 ClientSampleId :
 SV4

Tgt Ion: 43 Resp: 729




Ion	Ratio	Lower	Upper
43	100		
86	0.0	7.5	11.3#
42	48.1	8.4	12.6#
44	0.0	7.8	11.8#

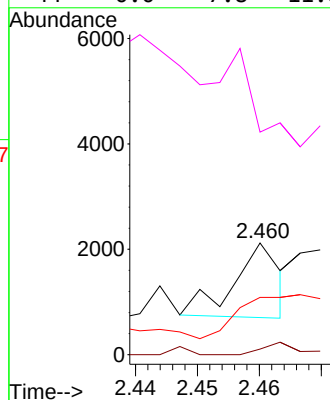


#25
 Ethyl Acetate
 Concen: 0.668 ppbv
 RT: 2.816 min Scan# 843
 Delta R.T. -0.003 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07

Tgt Ion: 43 Resp: 46640

Ion	Ratio	Lower	Upper
43	100		
45	0.5	8.3	12.5#
61	0.3	7.5	11.3#
70	1.8	6.8	10.2#


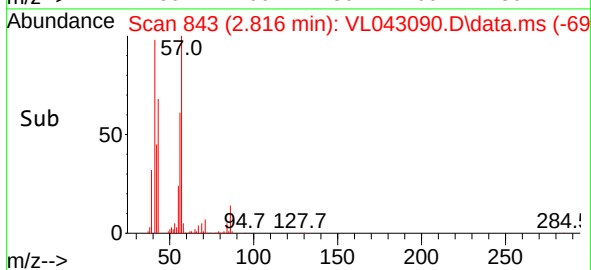
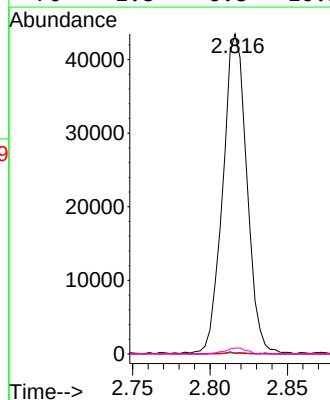





#26
Hexane
Concen: 2.410 ppbv
RT: 2.816 min Scan# 84
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 57 Resp: 64733
Ion Ratio Lower Upper
57 100
41 101.7 76.1 114.1
43 73.2 201.4 302.0#
56 61.4 44.0 66.0

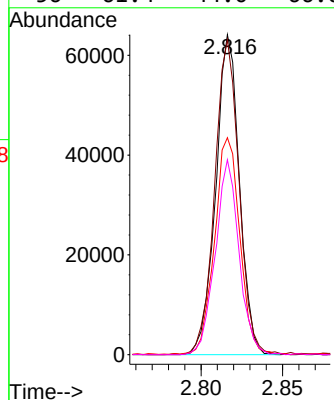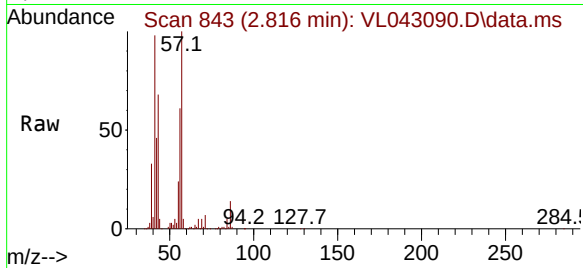

#27
Carbon Disulfide
Concen: 0.104 ppbv
RT: 2.140 min Scan# 634
Delta R.T. -0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 76 Resp: 3284
Ion Ratio Lower Upper
76 100
44 320.6 14.0 21.0#
78 19.4 9.4 14.0#


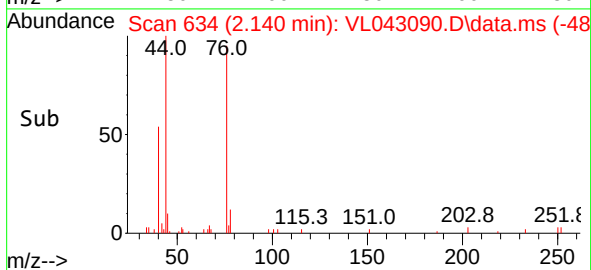
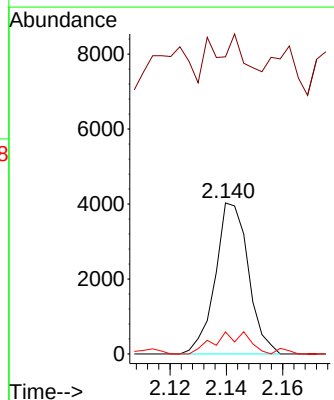
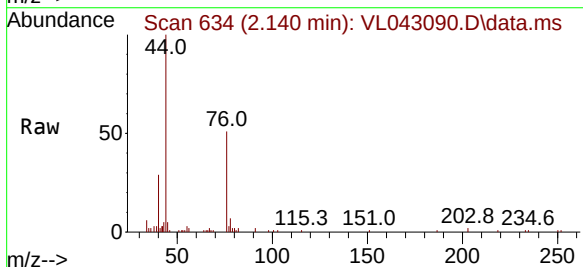


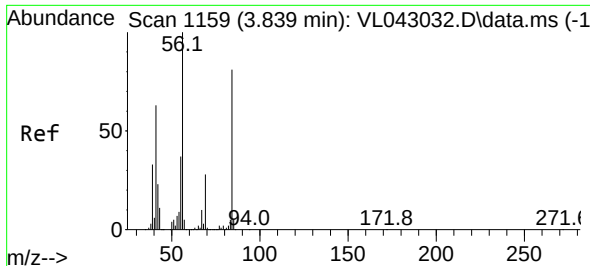

#30
Cyclohexane
Concen: 0.072 ppbv
RT: 3.836 min Scan# 1159
Delta R.T. -0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 84 Resp: 1599
Ion Ratio Lower Upper
84 100
56 165.0 99.9 149.9#
41 146.7 64.2 96.4#

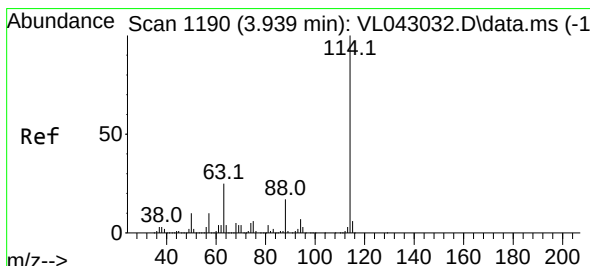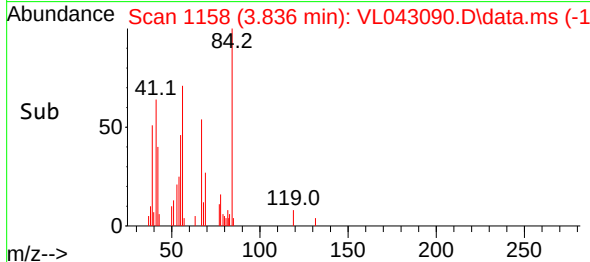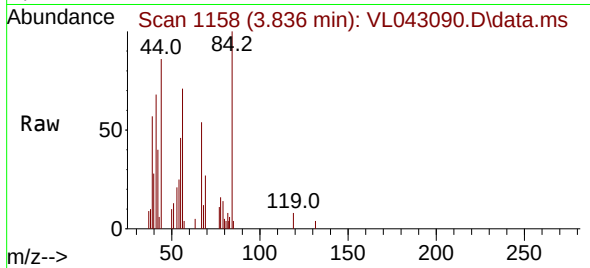

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.942 min Scan# 1191
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 114 Resp: 523879
Ion Ratio Lower Upper
114 100
63 25.6 19.4 29.2
88 17.6 13.9 20.9


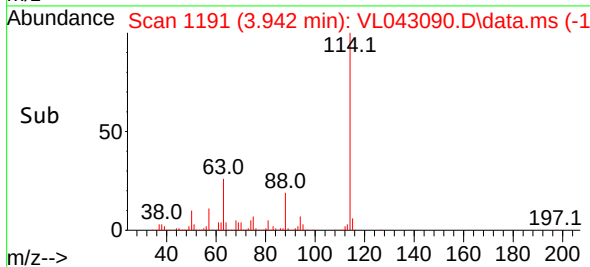

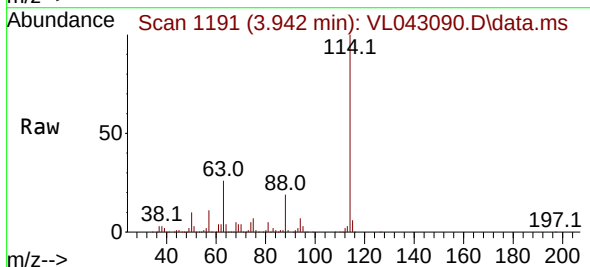




#34
2-Butanone
Concen: 0.421 ppbv
RT: 2.554 min Scan# 71
Delta R.T. 0.010 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 43 Resp: 14981
Ion Ratio Lower Upper
43 100
72 20.8 18.4 27.6

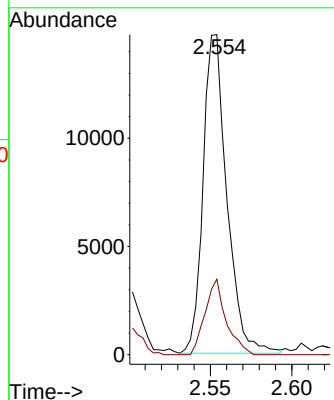

#36
Benzene
Concen: 0.043 ppbv
RT: 3.645 min Scan# 1099
Delta R.T. 0.007 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 78 Resp: 2146
Ion Ratio Lower Upper
78 100
77 19.9 19.2 28.8
50 17.7 14.9 22.3

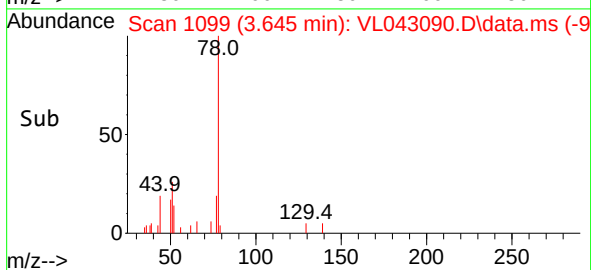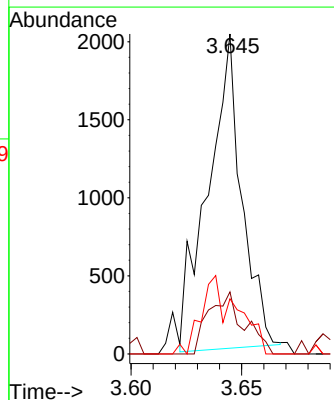







#38
 Trichloroethene
 Concen: 0.080 ppbv
 RT: 4.528 min Scan# 1191
 Delta R.T. 0.003 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07

Instrument :
 MSVOA_L
 ClientSampleId :
 SV4

Tgt Ion:130 Resp: 1672




Ion	Ratio	Lower	Upper
130	100		
95	97.2	86.4	129.6
132	49.7	75.7	113.5#
97	81.5	56.9	85.3

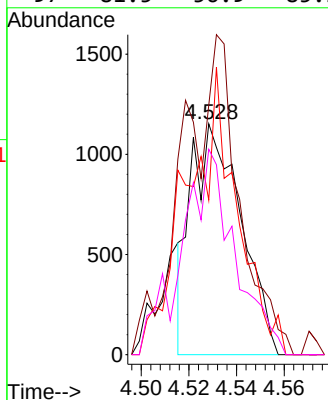


#39
 1,2-Dichloropropane
 Concen: 7.225 ppbv
 RT: 3.942 min Scan# 1191
 Delta R.T. -0.350 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07

Tgt Ion: 63 Resp: 134036

Ion	Ratio	Lower	Upper
63	100		
41	0.3	61.6	92.4#
62	17.2	58.1	87.1#

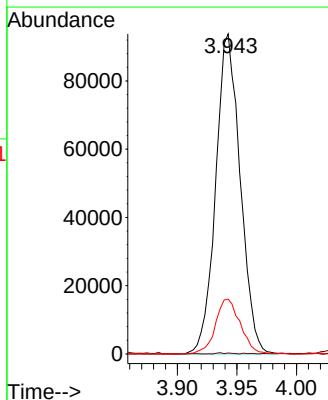



#41

Tetrahydrofuran

Concen: 0.128 ppbv

RT: 3.049 min Scan# 911

Delta R.T. 0.013 min

Lab File: VL043090.D

Acq: 09 Oct 2025 16:07





Instrument :

MSVOA_L

ClientSampleId :

SV4

Tgt Ion:	42	Resp:	2343
Ion	Ratio	Lower	Upper
42	100		
72	28.4	31.0	46.6#
71	21.0	29.8	44.6#

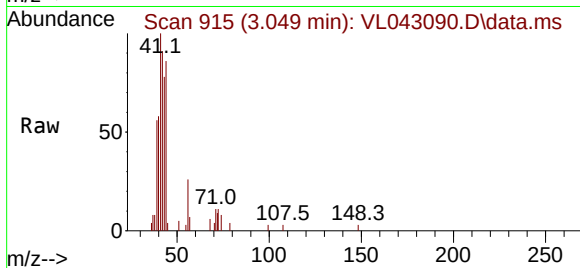

#51

2-Hexanone

Concen: 0.088 ppbv




RT: 7.409 min Scan# 2262


Delta R.T. -0.003 min

Lab File: VL043090.D

Acq: 09 Oct 2025 16:07

Tgt Ion:	43	Resp:	2707
Ion	Ratio	Lower	Upper
43	100		
58	0.0	39.1	58.7#
98	0.0	0.5	0.7#




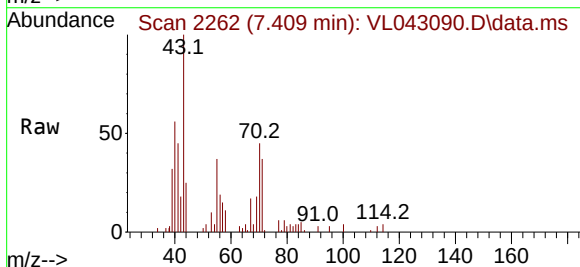




#52
Tetrachloroethene
Concen: 0.055 ppbv
RT: 8.215 min Scan# 2108
Delta R.T. 0.010 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion:164 Resp: 1021
Ion Ratio Lower Upper
164 100
166 115.0 101.8 152.8
129 94.2 84.5 126.7
131 76.6 80.9 121.3#

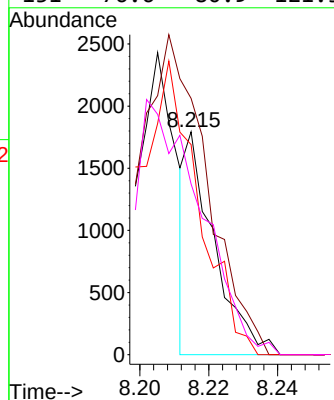

#53
Toluene
Concen: 0.424 ppbv
RT: 6.910 min Scan# 2108
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 91 Resp: 21425
Ion Ratio Lower Upper
91 100
92 59.3 47.8 71.6


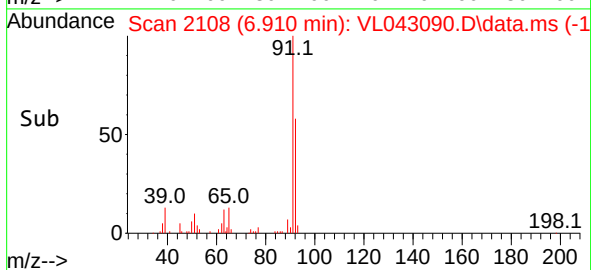
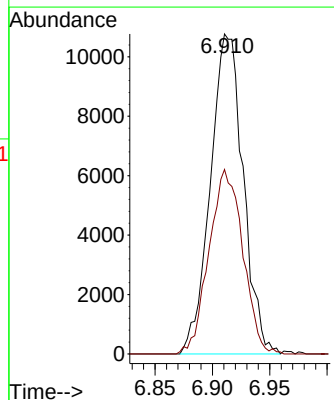





#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.865 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion:117 Resp: 525878
Ion Ratio Lower Upper
117 100
82 64.3 53.0 79.6
119 32.4 25.4 38.2



#58
Ethyl Benzene
Concen: 0.101 ppbv
RT: 9.341 min Scan# 2859
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 91 Resp: 8236
Ion Ratio Lower Upper
91 100
106 26.4 24.1 36.1


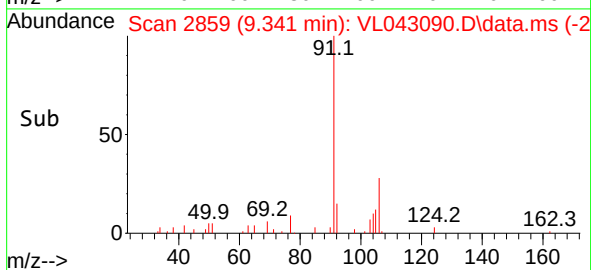






#59
m/p-Xylene
Concen: 0.037 ppbv
RT: 9.542 min Scan# 2918
Delta R.T. 0.010 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 2540
Ion Ratio Lower Upper
91 100
106 0.0 37.5 56.3#

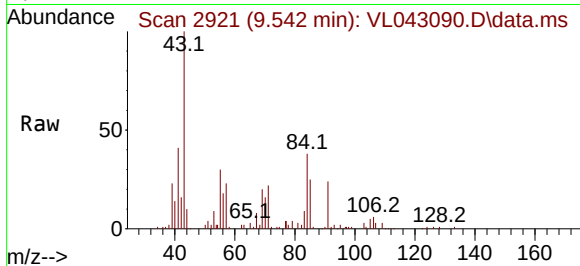

#60
o-Xylene
Concen: 0.183 ppbv
RT: 9.950 min Scan# 3047
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 91 Resp: 12540
Ion Ratio Lower Upper
91 100
106 39.3 21.9 65.5

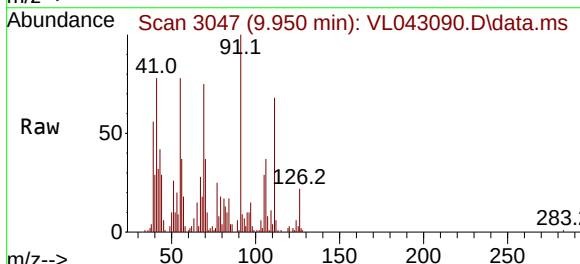



#63

1,1,2,2-Tetrachloroethane

Concen: 0.083 ppbv

RT: 9.934 min Scan# 3046

Delta R.T. -0.013 min

Lab File: VL043090.D

Acq: 09 Oct 2025 16:07

Instrument :

MSVOA_L

ClientSampleId :

SV4





Tgt Ion: 83 Resp: 4096

Ion Ratio Lower Upper

83 100

131 0.0 4.7 14.1#

85 69.9 32.0 96.2

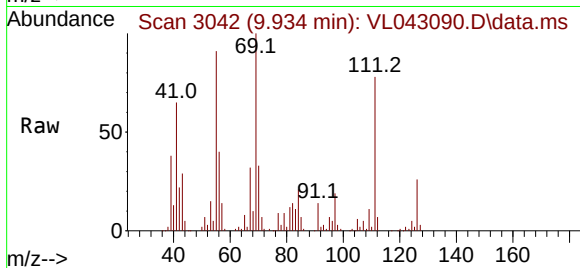

#64

n-propylbenzene

Concen: 0.033 ppbv

RT: 10.976 min Scan# 3364

Delta R.T. 0.000 min

Lab File: VL043090.D




Acq: 09 Oct 2025 16:07


Tgt Ion: 120 Resp: 888

Ion Ratio Lower Upper

120 100

91 902.7 367.0 550.4#


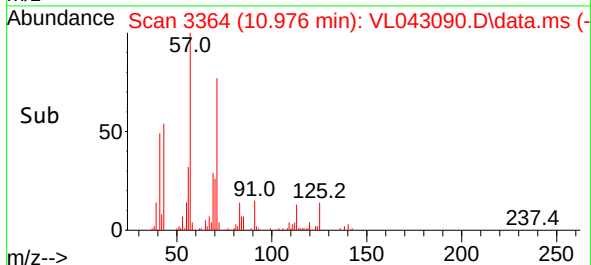

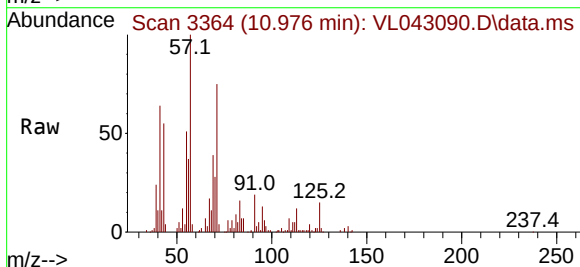




#66
Benzyl Chloride
Concen: 0.052 ppbv
RT: 11.623 min Scan# 3156
Delta R.T. 0.019 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 186
Ion Ratio Lower Upper
91 100
126 0.0 14.2 21.4#
128 0.0 4.8 7.2#

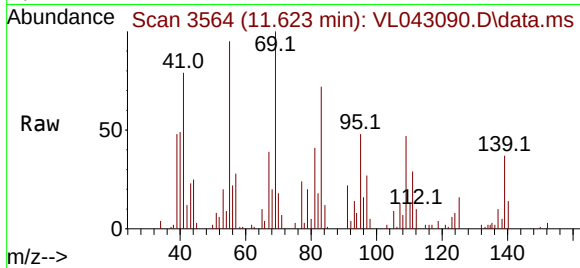

#68
1-Bromo-4-Fluorobenzene
Concen: 11.288 ppbv
RT: 10.364 min Scan# 3175
Delta R.T. 0.003 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 95 Resp: 427637
Ion Ratio Lower Upper
95 100
174 64.3 52.3 78.5
175 4.6 3.8 5.8


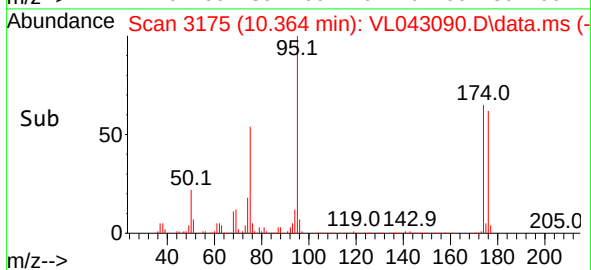

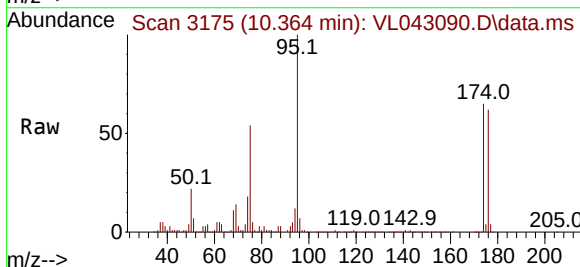


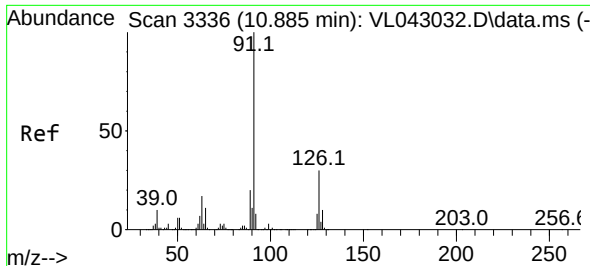

#71
2-Chlorotoluene
Concen: 0.044 ppbv
RT: 10.979 min Scan# 31
Delta R.T. 0.094 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 3370
Ion Ratio Lower Upper
91 100
126 26.3 12.2 48.6

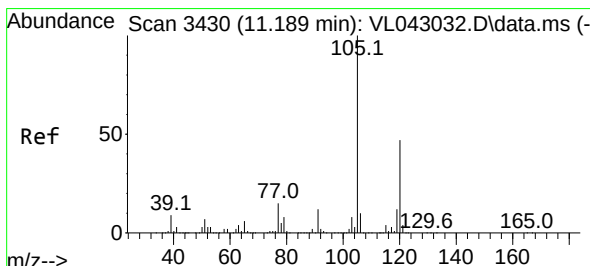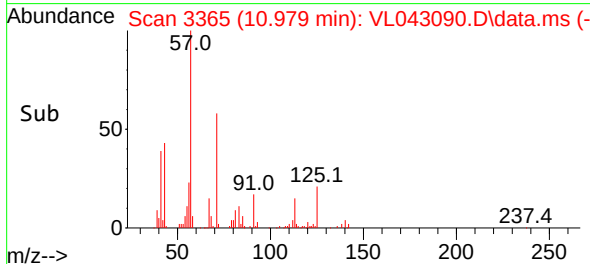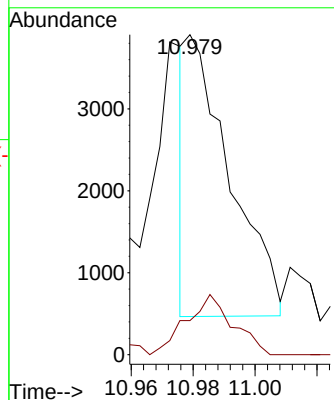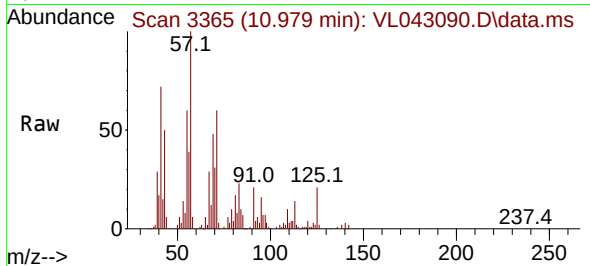

#73
1,3,5-Trimethylbenzene
Concen: 0.051 ppbv
RT: 11.189 min Scan# 3430
Delta R.T. 0.000 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion: 105 Resp: 3600
Ion Ratio Lower Upper
105 100
120 27.3 37.5 56.3#


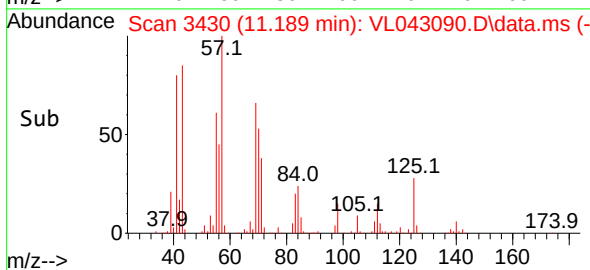
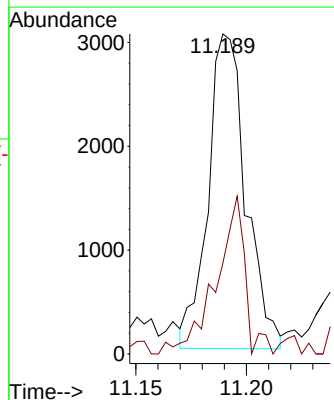
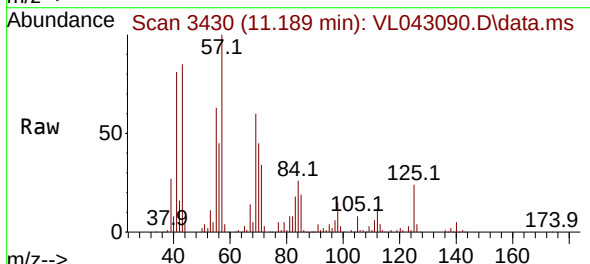




#74
1,2,4-Trimethylbenzene
Concen: 0.050 ppbv
RT: 11.523 min Scan# 31
Delta R.T. 0.000 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion:105	Resp:	3947
Ion Ratio	Lower	Upper
105	100	
120	56.9	39.7 59.5
91	5.6	56.5 84.7#
77	27.1	19.9 29.9

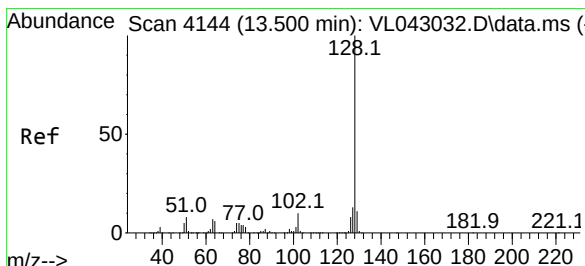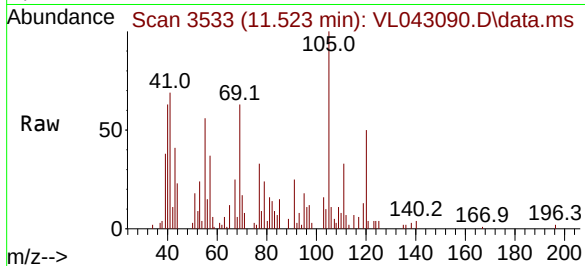

#79
Naphthalene
Concen: 0.240 ppbv
RT: 13.507 min Scan# 4146
Delta R.T. 0.007 min
Lab File: VL043090.D
Acq: 09 Oct 2025 16:07

Tgt Ion:128	Resp:	397
Ion Ratio	Lower	Upper
128	100	
127	34.3	10.6 16.0#
129	0.0	8.8 13.2#

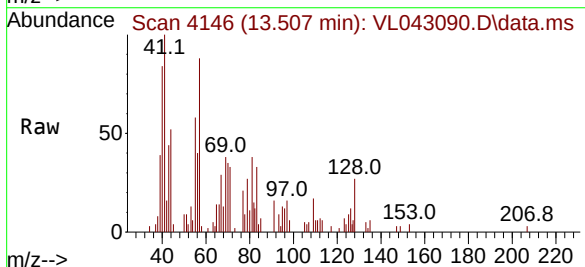

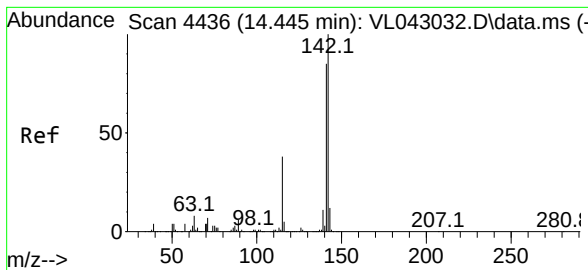

#80
 Naphthalene, 2-methyl-
 Concen: 0.682 ppbv
 RT: 14.452 min Scan# 44
 Delta R.T. 0.007 min
 Lab File: VL043090.D
 Acq: 09 Oct 2025 16:07

Instrument :
 MSVOA_L
 ClientSampleId :
 SV4

Tgt Ion:	142	Resp:	652
Ion	Ratio	Lower	Upper
142	100		
141	136.3	66.6	100.0#
115	84.2	30.1	45.1#

