
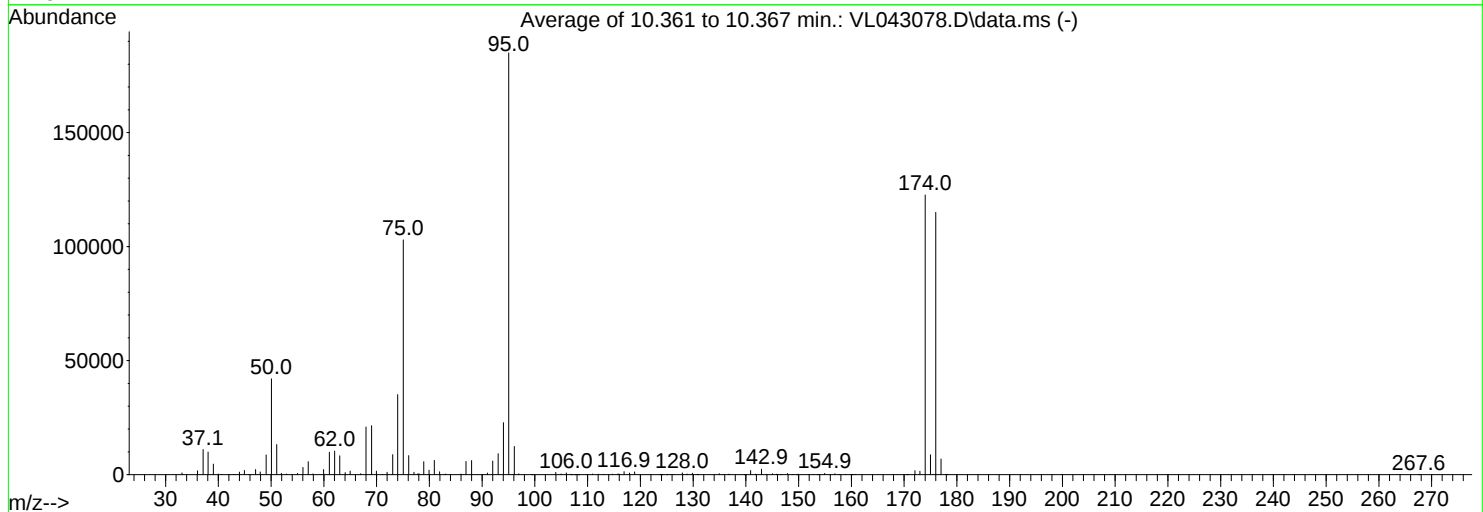


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL100925\
Data File : VL043078.D
Acq On : 09 Oct 2025 07:56
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL100225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Oct 03 08:23:34 2025

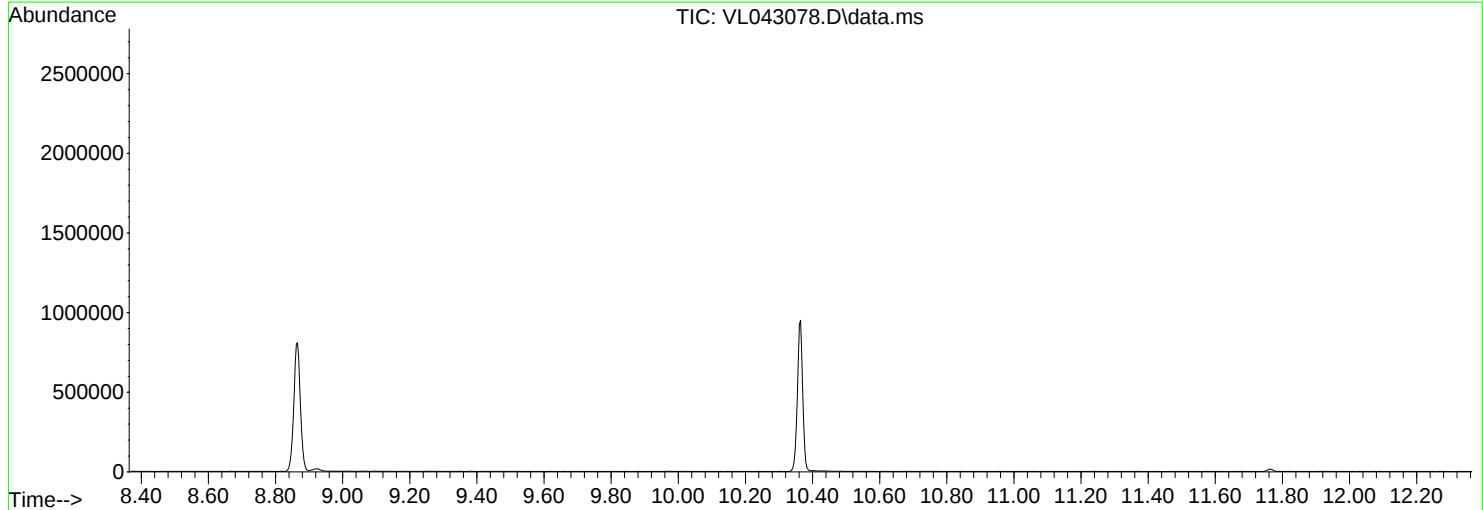

AutoFind: Scans 3174, 3175, 3176; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	42048	PASS
75	95	30	66	55.7	102957	PASS
95	95	100	100	100.0	184981	PASS
96	95	5	9	6.7	12353	PASS
173	174	0.00	2	1.2	1469	PASS
174	95	50	120	66.3	122685	PASS
175	174	4	9	7.1	8688	PASS
176	174	93	101	93.7	114976	PASS
177	176	5	9	6.0	6859	PASS

Average of 10.361 to 10.367 min.: VL043078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	815	44.95	1852	55.00	568	67.00	391
36.05	1673	45.75	82	56.05	3176	68.00	2089
37.10	11036	46.20	99	57.05	5677	69.05	2144
38.05	9897	47.05	2229	57.95	333	69.95	155
39.05	4635	47.95	1180	59.95	2221	71.15	72
40.00	319	49.05	8645	61.05	9799	72.00	1067
40.70	40	50.05	42048	62.05	10311	73.05	8785
41.90	31	51.05	13167	63.00	8279	74.00	35109
42.85	86	51.95	541	64.05	900	75.05	102957
43.15	84	52.95	314	65.00	1580	76.10	8344
44.00	1105	53.95	159	66.00	144	77.10	1092

Average of 10.361 to 10.367 min.: VL043078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.85	486	92.00	5974	107.00	28	116.90	1352
78.10	250	93.05	9225	107.60	30	117.95	735
78.95	5684	94.05	22789	108.00	31	118.90	1172
79.95	2005	95.05	184981	108.30	21	121.85	70
80.95	6225	96.10	12353	109.70	72	123.70	37
81.95	1279	96.95	344	110.95	252	123.90	72
83.00	280	99.40	25	112.05	199	124.10	35
86.00	293	103.95	979	113.00	150	125.00	26
86.95	5845	104.95	313	114.75	247	125.75	78
88.00	6180	105.95	783	115.75	330	126.30	49
91.00	682	106.80	200	116.00	212	127.95	797

Average of 10.361 to 10.367 min.: VL043078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.85	317	141.80	209	151.90	26	160.20	19
129.85	600	142.95	2363	152.75	110	160.70	77
130.80	122	143.85	154	153.60	19	160.85	152
131.00	110	145.05	455	154.00	109	170.50	20
134.95	456	145.85	194	154.95	595	170.80	173
135.65	58	146.60	69	155.90	46	172.05	1729
136.75	187	146.80	45	156.05	105	173.00	1469
137.00	152	147.90	527	156.90	430	174.00	122685
139.70	38	148.90	164	157.75	84	175.00	8688
140.00	61	149.60	32	158.95	163	176.00	114976
140.90	1857	150.00	191	159.90	38	177.00	6859

Average of 10.361 to 10.367 min.: VL043078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.90	160						
178.10	27						
267.60	19						

Instrument :

MSVOA_L

ClientSampleId :

BFB