
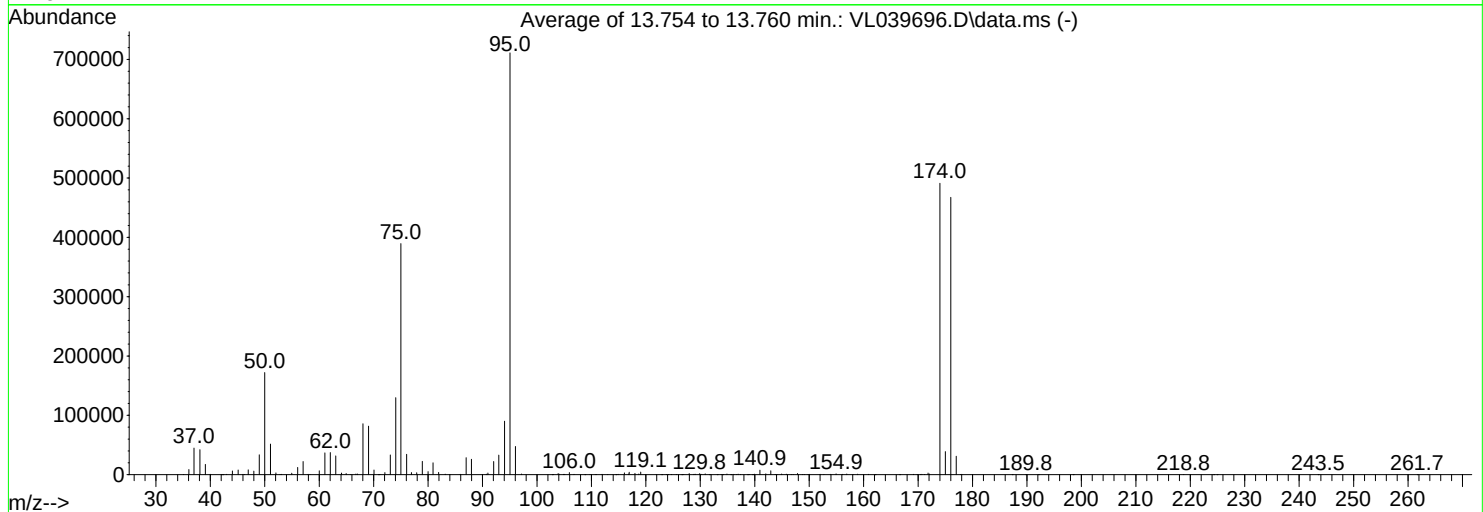


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101022\
Data File : VL039696.D
Acq On : 10 Oct 2022 12:38
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Sep 19 14:26:28 2022

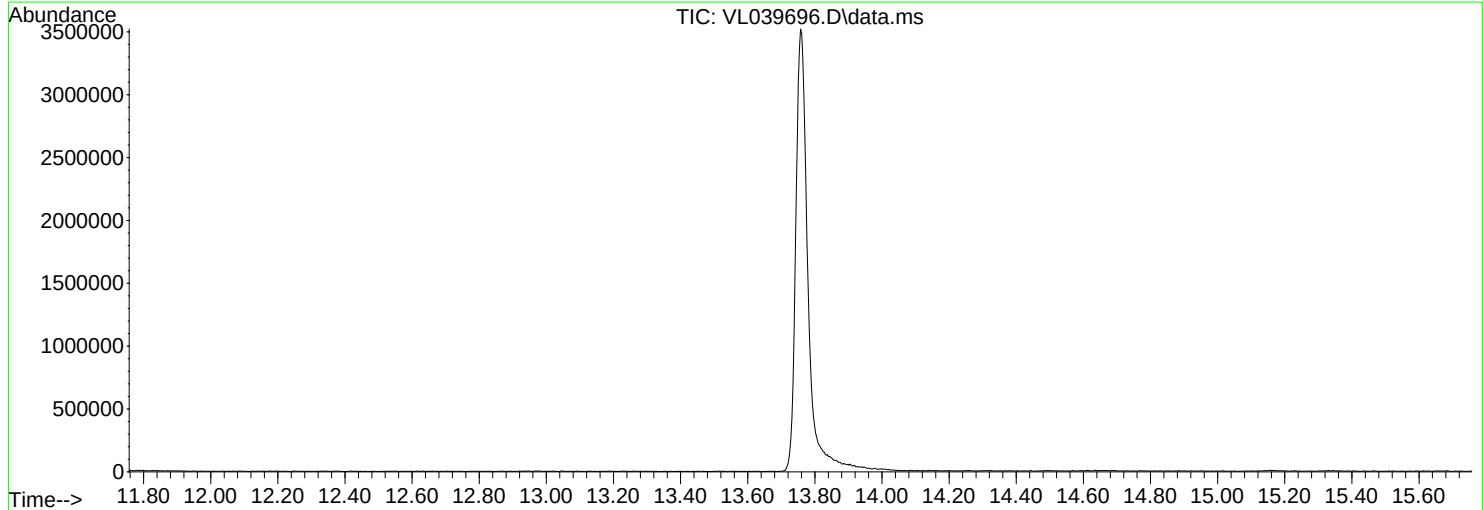

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	172245	PASS
75	95	30	66	54.8	389568	PASS
95	95	100	100	100.0	711040	PASS
96	95	5	9	6.7	47560	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.1	491307	PASS
175	174	4	9	7.9	38872	PASS
176	174	93	101	95.2	467499	PASS
177	176	5	9	6.6	30971	PASS

Average of 13.754 to 13.760 min.: VL039696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	166	46.00	520	56.05	12252	66.75	971
36.05	8745	46.30	338	57.05	22251	67.05	1083
37.00	44923	46.95	8127	57.95	531	68.05	8578
38.10	42232	48.00	5833	58.30	182	69.05	8169
39.10	17312	49.00	33427	60.00	6547	70.05	7872
40.00	458	50.00	172245	61.05	36597	70.90	129
42.00	59	51.05	51600	62.05	37243	71.15	379
42.30	105	52.05	2948	63.05	31517	72.05	3641
43.00	640	52.80	221	64.10	2808	73.05	33136
44.05	6162	53.05	422	64.95	1911	74.05	129792
45.10	7904	54.95	2379	65.80	267	75.00	389568

Average of 13.754 to 13.760 min.: VL039696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	34192	87.95	25891	103.90	1839	113.00	386
76.95	3438	90.70	756	104.10	815	114.50	95
77.90	3150	91.00	2703	104.85	682	114.90	597
78.95	22429	92.05	22227	105.10	440	116.05	2877
80.00	5082	93.00	32976	105.95	3562	116.80	1203
80.90	19960	94.05	90083	106.80	700	116.95	4049
81.95	3913	95.05	711040	108.80	79	118.00	2210
83.15	925	96.05	47560	109.75	178	118.70	1070
84.00	279	97.15	1121	110.70	253	119.05	4364
85.90	665	102.80	129	110.95	384	121.90	285
87.00	28722	103.05	186	111.95	679	122.90	107

Average of 13.754 to 13.760 min.: VL039696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.75	350	130.90	1357	138.70	114	145.80	706
124.15	384	131.70	53	139.05	276	146.70	252
124.70	160	133.10	119	139.60	87	147.05	186
125.60	209	133.85	171	139.95	807	147.85	1827
126.60	54	134.10	135	140.95	7706	148.80	333
126.95	404	134.90	964	142.05	1299	149.10	248
127.95	2022	135.60	64	142.95	6608	149.80	173
128.80	473	136.15	471	143.75	361	150.05	603
129.05	772	136.70	284	143.90	310	152.00	651
129.85	1598	136.95	841	144.10	258	152.70	400
130.10	950	137.40	163	144.95	1179	153.95	551

Average of 13.754 to 13.760 min.: VL039696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.95	1444	170.70	460	189.80	142		
156.15	529	171.20	369	192.10	67		
156.90	1227	171.85	2790	198.50	81		
158.05	221	172.10	1150	218.80	168		
158.90	895	174.00	491307	224.30	51		
160.90	623	175.00	38872	224.90	56		
162.10	92	176.00	467499	243.50	106		
166.60	62	177.00	30971	261.70	56		
169.15	650	177.80	338				
169.85	167	178.05	550				
170.45	352	187.30	87				