


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL101620\
 Data File : VL035781.D
 Acq On : 16 Oct 2020 10:25
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL092320AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 23 07:38:05 2020
 Last Update : Wed Sep 23 07:38:05 2020

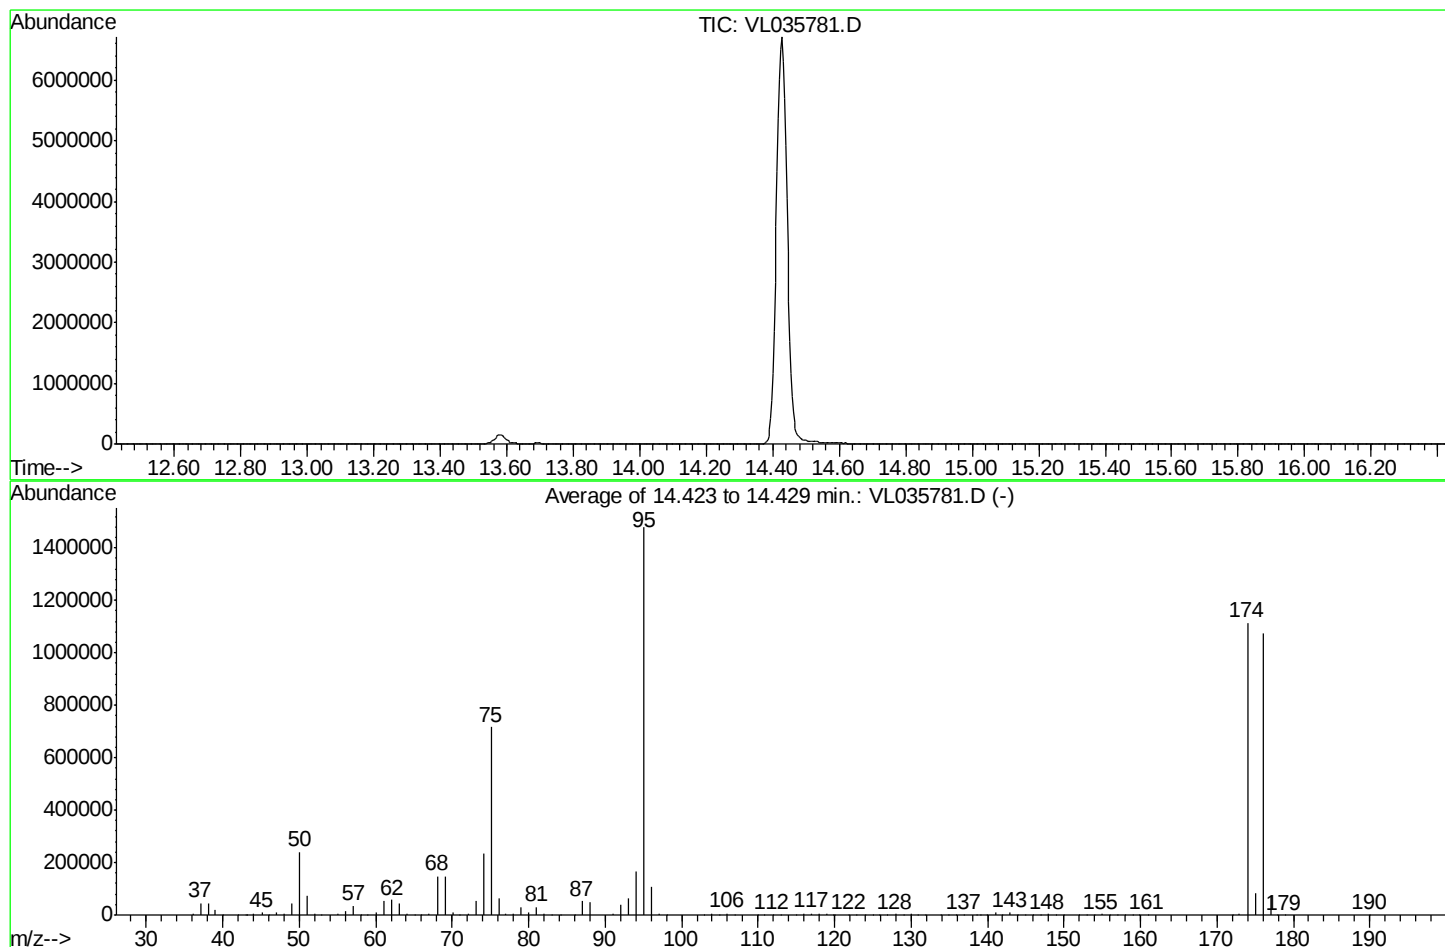

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	16.2	239317	PASS
75	95	30	66	48.5	716992	PASS
95	95	100	100	100.0	1478826	PASS
96	95	5	9	7.3	107437	PASS
173	174	0.00	2	0.5	6096	PASS
174	95	50	120	75.4	1115136	PASS
175	174	4	9	7.4	82709	PASS
176	174	93	101	96.5	1075968	PASS
177	176	5	9	7.0	75112	PASS