

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101625\
 Data File : VL043126.D
 Acq On : 16 Oct 2025 10:26
 Operator : SY/MD
 Sample : Q3247-01DL 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 RR-VOAS-AIRDL

Quant Time: Oct 17 01:12:43 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Oct 15 02:12:58 2025
 Response via : Initial Calibration


Compound		R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards							
1) Bromochloromethane		2.793	49	90785	10.000	ppbv	0.00
33) 1,4-Difluorobenzene		3.968	114	286778	10.000	ppbv	0.00
55) Chlorobenzene-d5		8.888	117	249452	10.000	ppbv	0.00
System Monitoring Compounds							
68) 1-Bromo-4-Fluorobenzene		10.380	95	207856	10.720	ppbv	0.00
Spiked Amount		10.000	Range 65 - 135		Recovery	= 107.200%	
Target Compounds							Qvalue
5) Vinyl Chloride		1.586	62	170	0.034	ppbv #	81
13) Ethanol		1.774	45	178	0.078	ppbv #	38
15) Acetone		1.842	43	1177	0.096	ppbv	99
18) 1,1-Dichloroethene		2.347	96	27009	6.095	ppbv	87
20) Methylene Chloride		2.068	84	1389	0.287	ppbv #	86
22) trans-1,2-Dichloroethene		2.347	96	27009	5.099	ppbv	86
24) 1,1-Dichloroethane		2.415	63	86684	8.471	ppbv	98
29) Chloroform		2.855	83	311004	15.351	ppbv	99
31) cis-1,2-Dichloroethene		2.729	61	129758	9.718	ppbv	94
36) Benzene		3.664	78	55384	2.050	ppbv	99
37) 1,2-Dichloroethane		3.224	62	183305	11.781	ppbv	97
38) Trichloroethene		4.557	130	5378	0.477	ppbv	94
39) 1,2-Dichloropropane		4.321	63	49492	5.012	ppbv	88
47) 1,1,2-Trichloroethane		6.590	97	74016	6.941	ppbv	95
52) Tetrachloroethene		8.231	164	99913	10.258	ppbv	95
53) Toluene		6.943	91	176460	5.505	ppbv	98
58) Ethyl Benzene		9.361	91	339931	7.940	ppbv	96
59) m/p-Xylene		9.558	91	541661	15.863	ppbv	96
60) o-Xylene		9.969	91	116992	3.469	ppbv	98
61) Styrene		9.966	104	2446	0.161	ppbv #	1
63) 1,1,2,2-Tetrachloroethane		9.969	83	108714	4.814	ppbv	99
64) n-propylbenzene		11.209	120	282142	17.488	ppbv #	1
65) tert-Butylbenzene		11.542	119	42919	0.798	ppbv #	56
66) Benzyl Chloride		11.542	91	50336	8.404	ppbv #	65
67) sec-Butylbenzene		11.542	105	407966	5.342	ppbv #	57
69) p-Isopropyltoluene		11.542	119	42991	0.662	ppbv #	1
71) 2-Chlorotoluene		11.209	91	79082	1.701	ppbv #	45
72) 4-Ethyltoluene		11.209	105	646782	15.597	ppbv #	86
73) 1,3,5-Trimethylbenzene		11.209	105	646782	18.912	ppbv	93
74) 1,2,4-Trimethylbenzene		11.542	105	407966	10.660	ppbv #	49
75) 1,3-Dichlorobenzene		11.613	146	131803	5.938	ppbv	99
76) 1,4-Dichlorobenzene		11.678	146	217615	9.723	ppbv	97
77) 1,2-Dichlorobenzene		11.678	146	217615	10.134	ppbv	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 17 01:12:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Wed Oct 15 02:12:58 2025
Response via : Initial Calibration









#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.793 min Scan# 835
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 49 Resp: 90785
Ion Ratio Lower Upper
49 100
128 51.0 24.4 73.4
130 65.1 31.0 93.0



#5
Vinyl Chloride
Concen: 0.034 ppbv
RT: 1.586 min Scan# 463
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 62 Resp: 170
Ion Ratio Lower Upper
62 100
64 20.1 24.6 36.8#


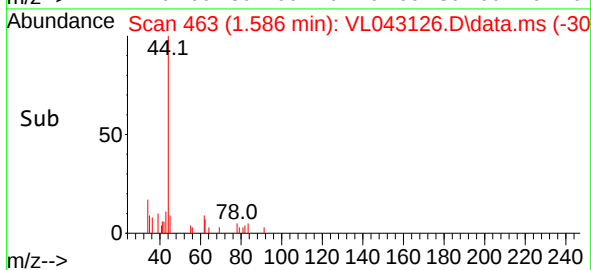






#13
 Ethanol
 Concen: 0.078 ppbv
 RT: 1.774 min Scan# 51
 Delta R.T. 0.052 min
 Lab File: VL043126.D
 Acq: 16 Oct 2025 10:26




Instrument :
 MSVOA_L
 ClientSampleId :
 RR-VOAS-AIRDL


Tgt Ion: 45 Resp: 178
 Ion Ratio Lower Upper
 45 100
 46 0.0 14.7 58.9#



#15
 Acetone
 Concen: 0.096 ppbv
 RT: 1.842 min Scan# 542
 Delta R.T. 0.006 min
 Lab File: VL043126.D
 Acq: 16 Oct 2025 10:26

Tgt Ion: 43 Resp: 1177
 Ion Ratio Lower Upper
 43 100
 58 25.5 20.8 31.2


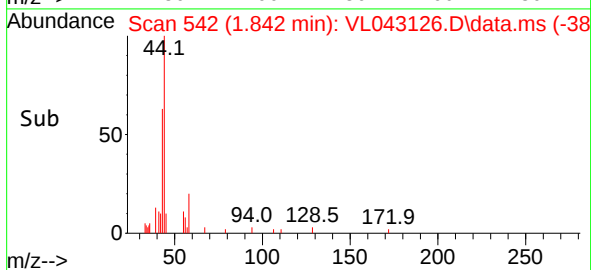






#18
1,1-Dichloroethene
Concen: 6.095 ppbv
RT: 2.347 min Scan# 61
Delta R.T. 0.310 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 96 Resp: 27009
Ion Ratio Lower Upper
96 100
61 190.9 173.4 260.0
98 67.0 53.2 79.8

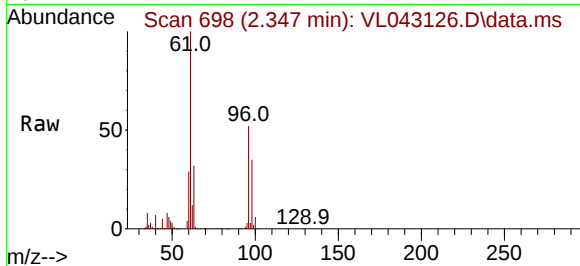

#20
Methylene Chloride
Concen: 0.287 ppbv
RT: 2.068 min Scan# 612
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 84 Resp: 1389
Ion Ratio Lower Upper
84 100
49 163.8 116.6 175.0
51 44.9 34.8 52.2
86 73.1 46.2 69.4




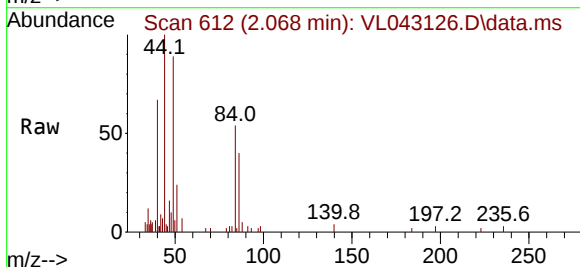




#22
trans-1,2-Dichloroethene
Concen: 5.099 ppbv
RT: 2.347 min Scan# 697
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 96 Resp: 27009
Ion Ratio Lower Upper
96 100
61 190.9 137.0 205.6
98 67.0 45.5 68.3

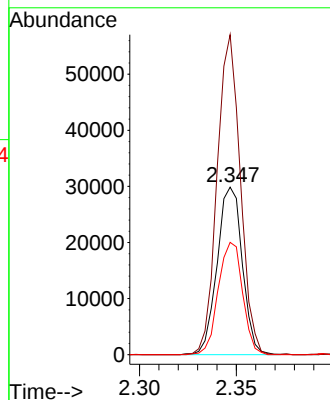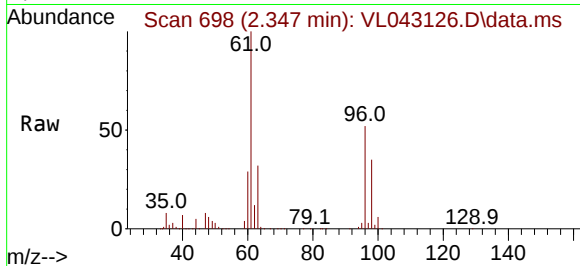

#24
1,1-Dichloroethane
Concen: 8.471 ppbv
RT: 2.415 min Scan# 719
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 63 Resp: 86684
Ion Ratio Lower Upper
63 100
98 4.1 2.6 7.8
100 3.1 1.5 4.4

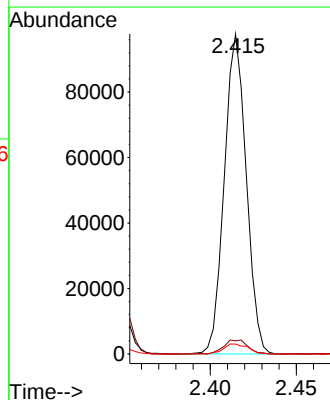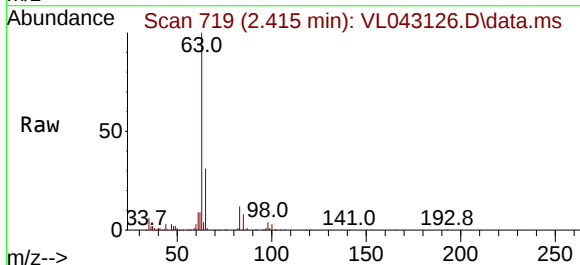



#29

Chloroform

Concen: 15.351 ppbv

RT: 2.855 min Scan# 81

Delta R.T. 0.003 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26

Instrument :

MSVOA_L

ClientSampleId :





RR-VOAS-AIRDL

Tgt Ion: 83 Resp: 311004

Ion Ratio Lower Upper

83 100

85 63.8 51.8 77.6

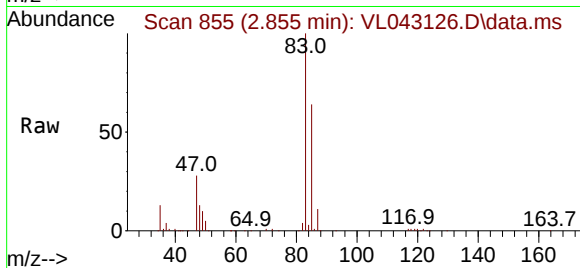

#31

cis-1,2-Dichloroethene

Concen: 9.718 ppbv

RT: 2.729 min Scan# 816

Delta R.T. 0.006 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26




Tgt Ion: 61 Resp: 129758


Ion Ratio Lower Upper

61 100

96 70.3 51.0 76.6

98 44.2 33.5 50.3

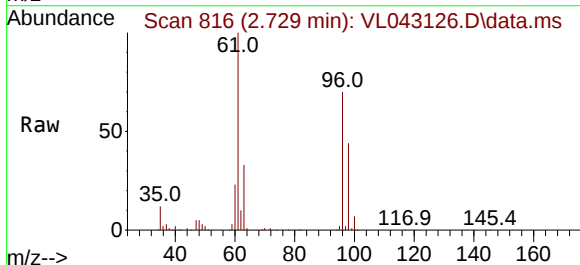



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 3.968 min Scan# 1199

Delta R.T. 0.006 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26

Instrument :

MSVOA_L

ClientSampleId :

RR-VOAS-AIRDL





Tgt Ion:114 Resp: 286778

Ion Ratio Lower Upper

114 100

63 25.2 19.3 28.9

88 17.9 13.9 20.9

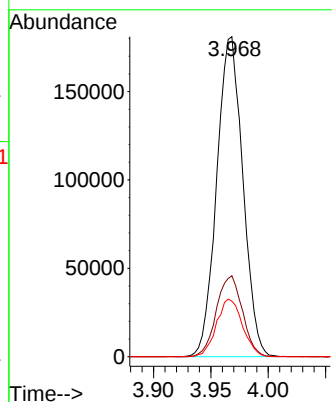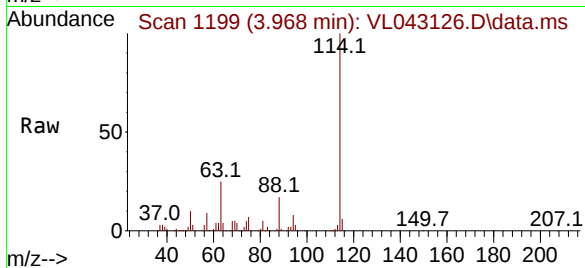

#36

Benzene

Concen: 2.050 ppbv

RT: 3.664 min Scan# 1105

Delta R.T. 0.003 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26




Tgt Ion: 78 Resp: 55384


Ion Ratio Lower Upper

78 100

77 21.1 17.0 25.6

50 18.6 14.6 22.0




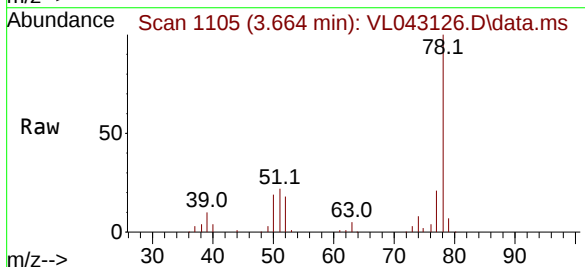




#37
1,2-Dichloroethane
Concen: 11.781 ppbv
RT: 3.224 min Scan# 90
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 62 Resp: 183305
Ion Ratio Lower Upper
62 100
98 6.2 5.8 8.6

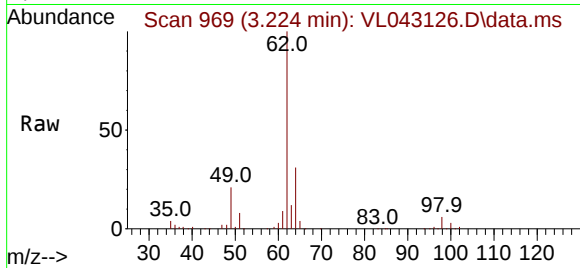

#38
Trichloroethene
Concen: 0.477 ppbv
RT: 4.557 min Scan# 1381
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion:130 Resp: 5378
Ion Ratio Lower Upper
130 100
95 115.4 88.6 133.0
132 101.5 73.4 110.0
97 76.0 57.8 86.6

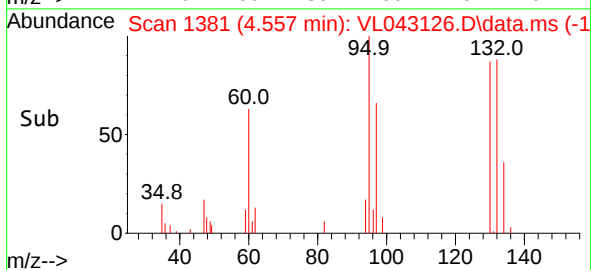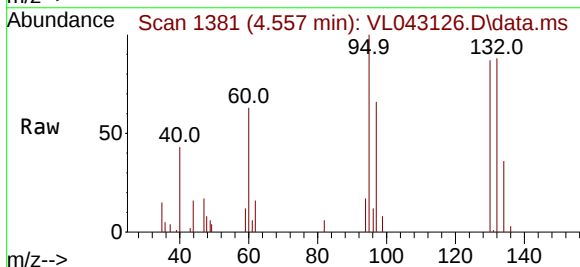



#39

1,2-Dichloropropane

Concen: 5.012 ppbv

RT: 4.321 min Scan# 11

Delta R.T. 0.006 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26

Instrument :

MSVOA_L

ClientSampleId :

RR-VOAS-AIRDL





Tgt Ion: 63 Resp: 49492

Ion Ratio Lower Upper

63 100

41 85.8 58.0 87.0

62 74.9 54.7 82.1

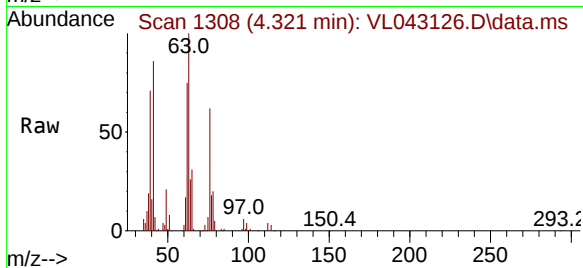

#47

1,1,2-Trichloroethane

Concen: 6.941 ppbv

RT: 6.590 min Scan# 2009

Delta R.T. 0.006 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26

Tgt Ion: 97 Resp: 74016




Ion Ratio Lower Upper


97 100

83 77.3 64.6 96.8

85 54.9 40.6 60.8

99 57.4 48.4 72.6




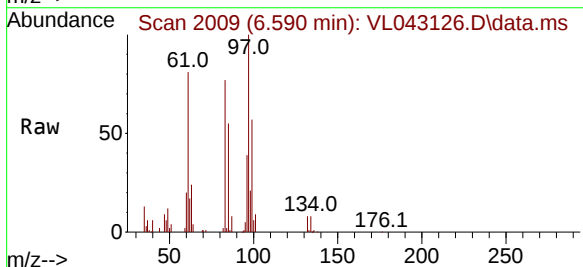




#52
Tetrachloroethene
Concen: 10.258 ppbv
RT: 8.231 min Scan# 2117
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion:164 Resp: 99913
Ion Ratio Lower Upper
164 100
166 115.7 97.6 146.4
129 108.2 84.5 126.7
131 102.3 77.2 115.8

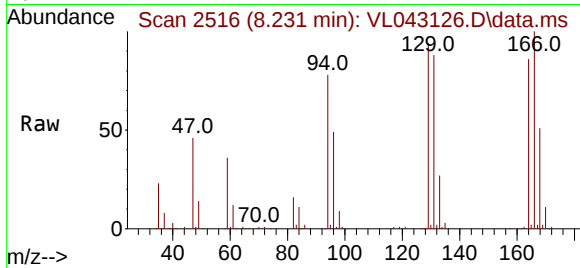

#53
Toluene
Concen: 5.505 ppbv
RT: 6.943 min Scan# 2118
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 91 Resp: 176460
Ion Ratio Lower Upper
91 100
92 59.7 48.8 73.2


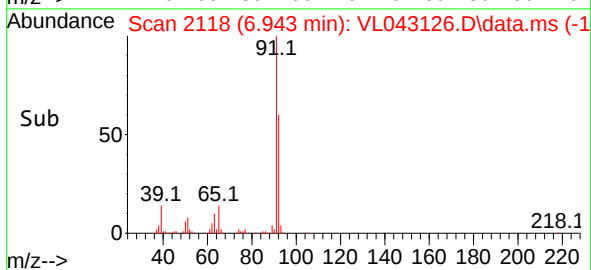

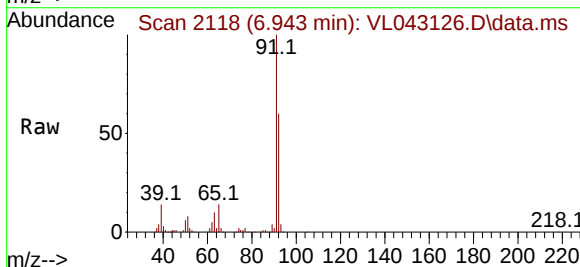




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.888 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion:117 Resp: 249452
Ion Ratio Lower Upper
117 100
82 66.3 53.8 80.8
119 32.0 25.4 38.0



#58
Ethyl Benzene
Concen: 7.940 ppbv
RT: 9.361 min Scan# 2865
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 91 Resp: 339931
Ion Ratio Lower Upper
91 100
106 28.7 24.8 37.2


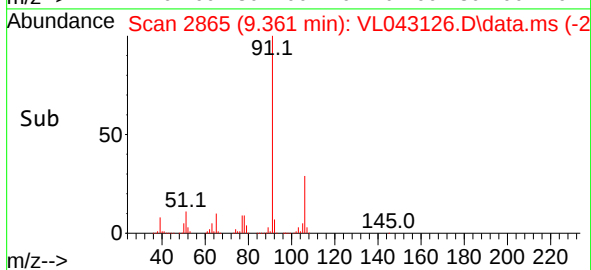






#59
m/p-Xylene
Concen: 15.863 ppbv
RT: 9.558 min Scan# 2919
Delta R.T. 0.022 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 91 Resp: 541661
Ion Ratio Lower Upper
91 100
106 44.9 38.0 57.0

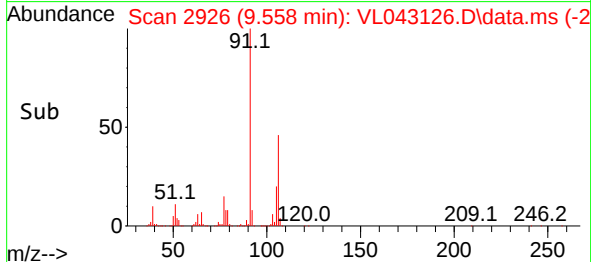

#60
o-Xylene
Concen: 3.469 ppbv
RT: 9.969 min Scan# 3053
Delta R.T. -0.000 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 91 Resp: 116992
Ion Ratio Lower Upper
91 100
106 42.3 21.9 65.8


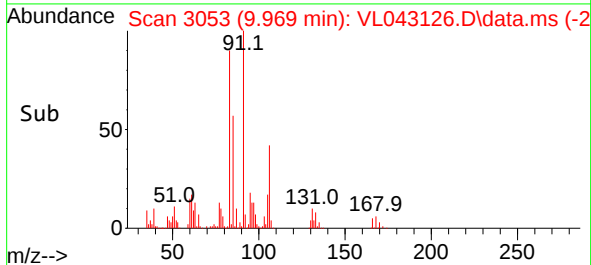






#61
Styrene
Concen: 0.161 ppbv
RT: 9.966 min Scan# 3052
Delta R.T. 0.090 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion:104 Resp: 2446
Ion Ratio Lower Upper
104 100
78 400.7 40.2 60.2#
103 286.3 36.9 55.3#

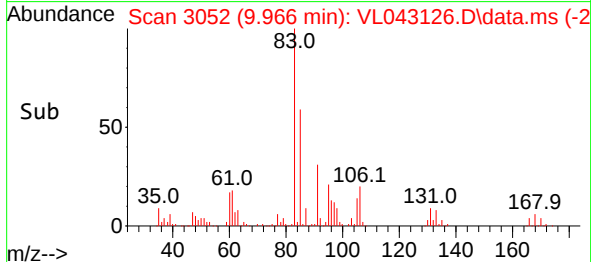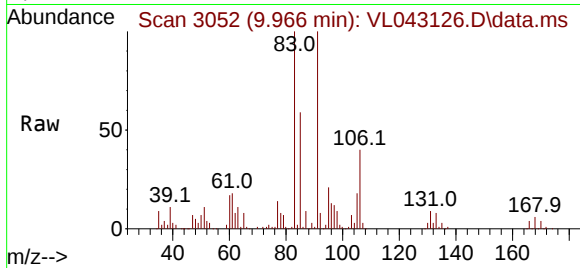

#63
1,1,2,2-Tetrachloroethane
Concen: 4.814 ppbv
RT: 9.969 min Scan# 3053
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 83 Resp: 108714
Ion Ratio Lower Upper
83 100
131 9.8 4.8 14.3
85 63.4 32.0 96.0




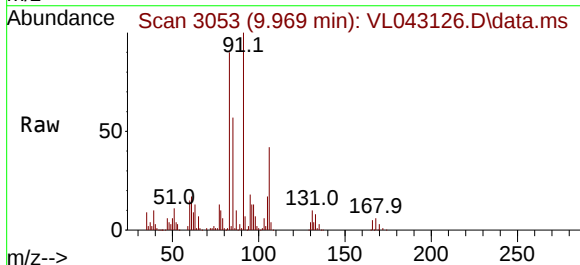




#64
n-propylbenzene
Concen: 17.488 ppbv
RT: 11.209 min Scan# 34
Delta R.T. 0.217 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion:120 Resp: 282142
Ion Ratio Lower Upper
120 100
91 28.2 361.6 542.4#



#65
tert-Butylbenzene
Concen: 0.798 ppbv
RT: 11.542 min Scan# 3539
Delta R.T. 0.006 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion:119 Resp: 42919
Ion Ratio Lower Upper
119 100
91 117.3 63.4 95.0#
134 0.1 17.3 25.9#

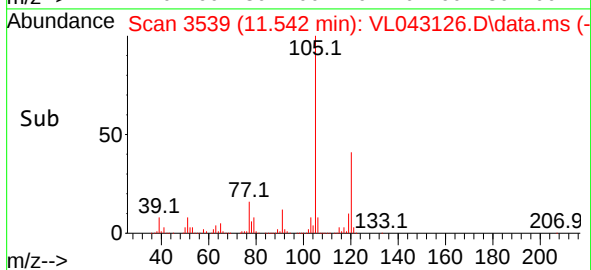

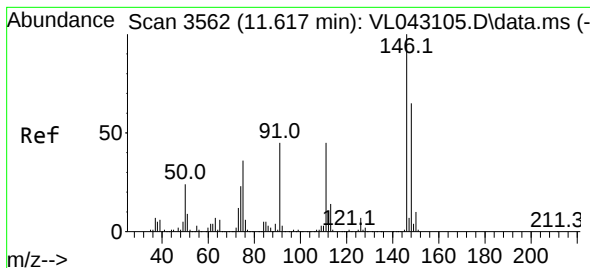

#66

Benzyl Chloride

Concen: 8.404 ppbv

RT: 11.542 min Scan# 3539

Delta R.T. -0.075 min

Lab File: VL043126.D

Acq: 16 Oct 2025 10:26

Instrument :

MSVOA_L

ClientSampleId :

RR-VOAS-AIRDL





Tgt Ion: 91 Resp: 50336

Ion Ratio Lower Upper

91 100

126 0.0 14.6 22.0#

128 0.0 4.6 6.8#

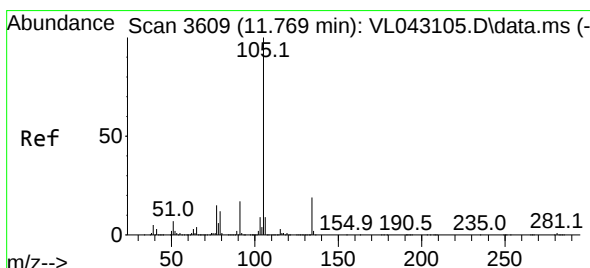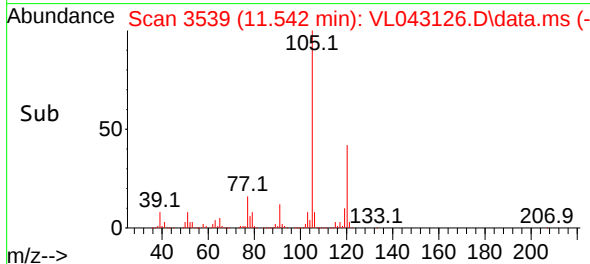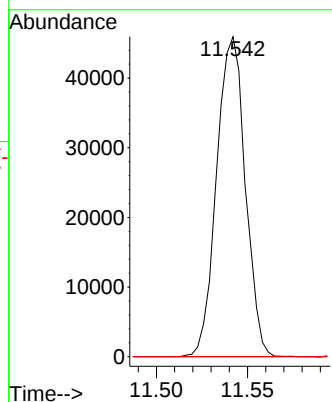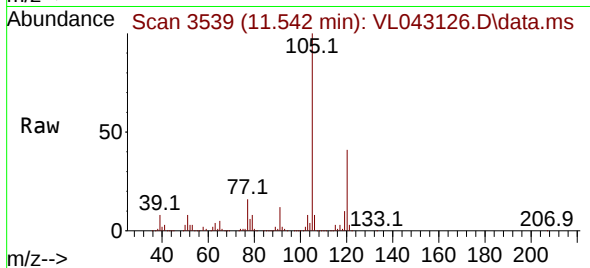

#67

sec-Butylbenzene

Concen: 5.342 ppbv

RT: 11.542 min Scan# 3539

Delta R.T. -0.227 min

Lab File: VL043126.D




Acq: 16 Oct 2025 10:26


Tgt Ion: 105 Resp: 407966

Ion Ratio Lower Upper

105 100

134 0.0 15.5 23.3#


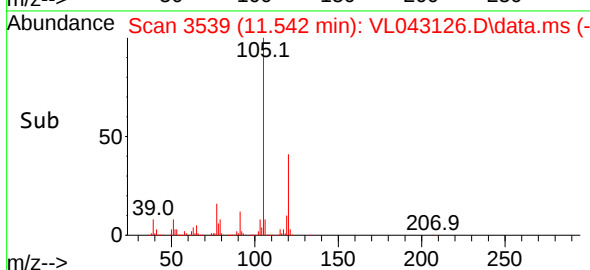

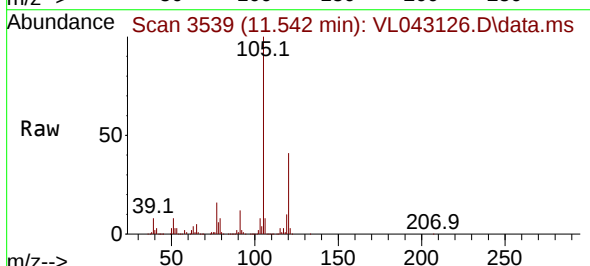




#68
1-Bromo-4-Fluorobenzene
Concen: 10.720 ppbv
RT: 10.380 min Scan# 3180
Delta R.T. -0.000 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 95 Resp: 207856
Ion Ratio Lower Upper
95 100
174 57.1 48.3 72.5
175 4.2 3.8 5.8

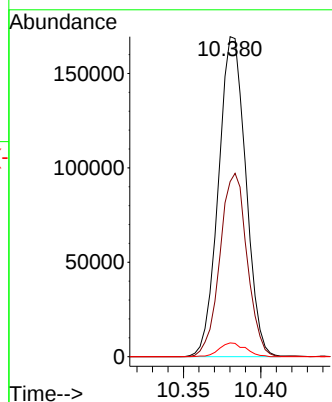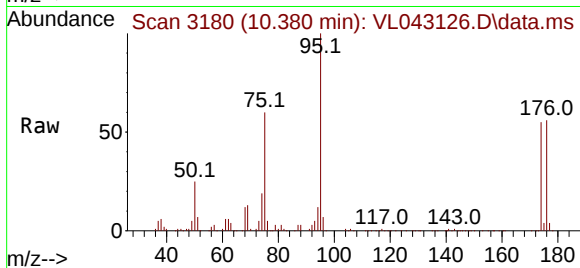

#69
p-Isopropyltoluene
Concen: 0.662 ppbv
RT: 11.542 min Scan# 3539
Delta R.T. -0.385 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion: 119 Resp: 42991
Ion Ratio Lower Upper
119 100
134 0.1 20.3 30.5#
91 117.1 22.6 33.8#




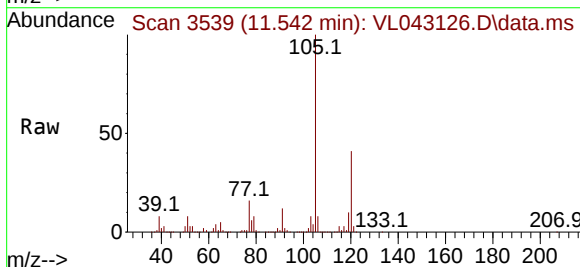


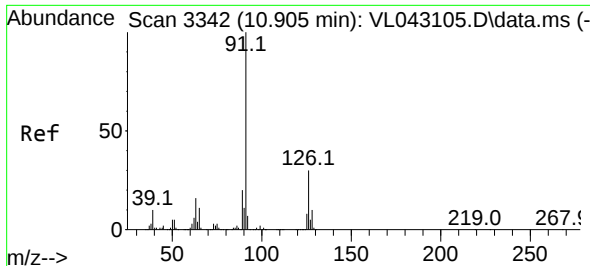

#71
2-Chlorotoluene
Concen: 1.701 ppbv
RT: 11.209 min Scan# 3436
Delta R.T. 0.304 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion: 91 Resp: 79082
Ion Ratio Lower Upper
91 100
126 0.0 12.0 48.0#

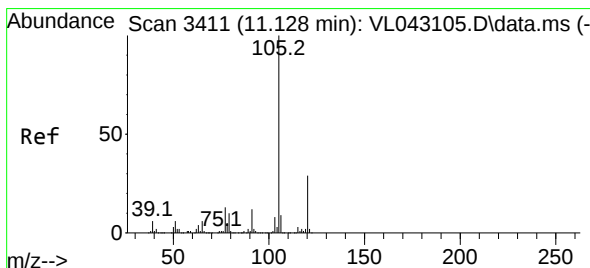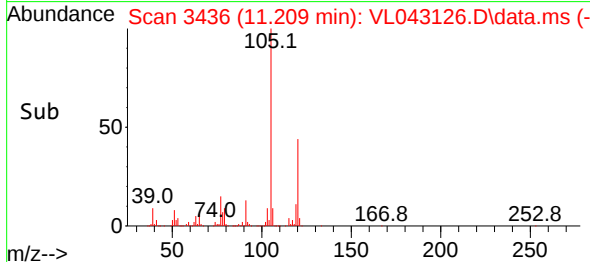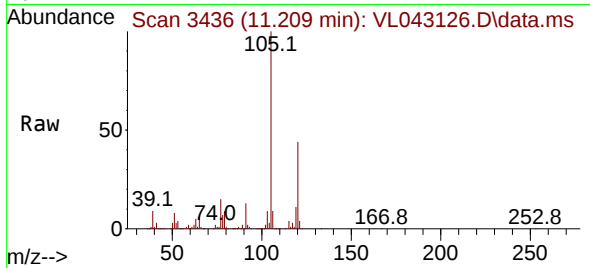

#72
4-Ethyltoluene
Concen: 15.597 ppbv
RT: 11.209 min Scan# 3436
Delta R.T. 0.081 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion:105 Resp: 646782
Ion Ratio Lower Upper
105 100
120 43.6 24.2 36.4#
91 12.3 10.0 15.0
77 15.2 10.7 16.1


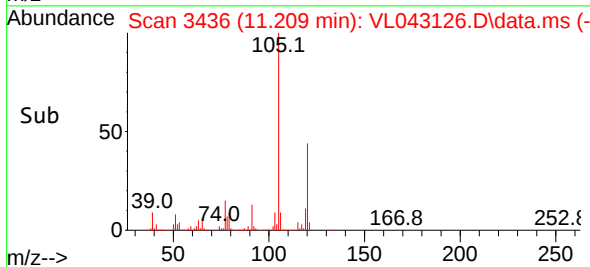

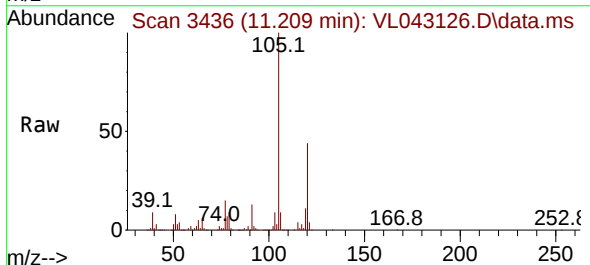




#73
1,3,5-Trimethylbenzene
Concen: 18.912 ppbv
RT: 11.209 min Scan# 3436
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion:105 Resp: 646782
Ion Ratio Lower Upper
105 100
120 44.2 39.0 58.6

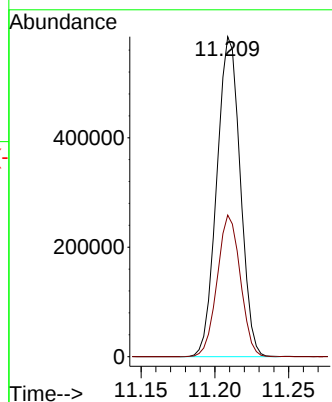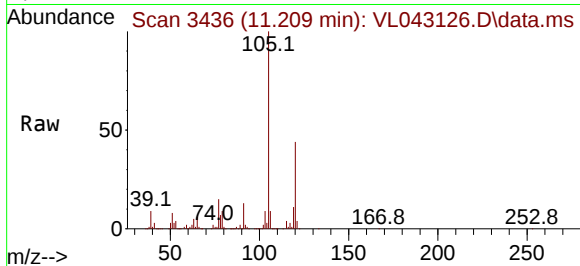

#74
1,2,4-Trimethylbenzene
Concen: 10.660 ppbv
RT: 11.542 min Scan# 3539
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion:105 Resp: 407966
Ion Ratio Lower Upper
105 100
120 41.5 42.8 64.2#
91 11.8 68.3 102.5#
77 15.7 23.4 35.0#




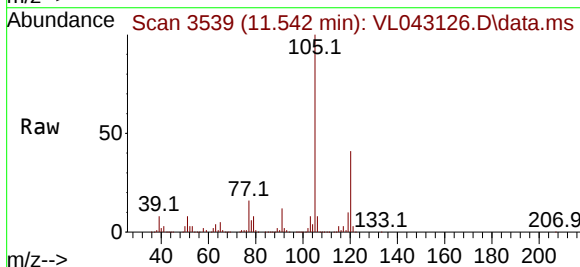




#75
1,3-Dichlorobenzene
Concen: 5.938 ppbv
RT: 11.613 min Scan# 3561
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26




Instrument :
MSVOA_L
ClientSampleId :
RR-VOAS-AIRDL


Tgt Ion:146 Resp: 131803
Ion Ratio Lower Upper
146 100
111 47.5 23.3 69.9
148 62.2 31.6 95.0

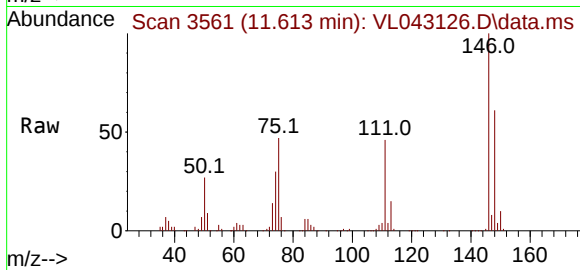

#76
1,4-Dichlorobenzene
Concen: 9.723 ppbv
RT: 11.678 min Scan# 3581
Delta R.T. 0.003 min
Lab File: VL043126.D
Acq: 16 Oct 2025 10:26

Tgt Ion:146 Resp: 217615
Ion Ratio Lower Upper
146 100
111 46.5 22.4 67.0
148 65.4 31.6 94.7

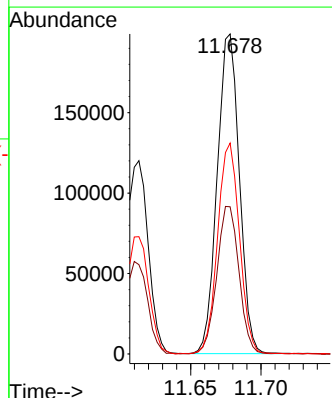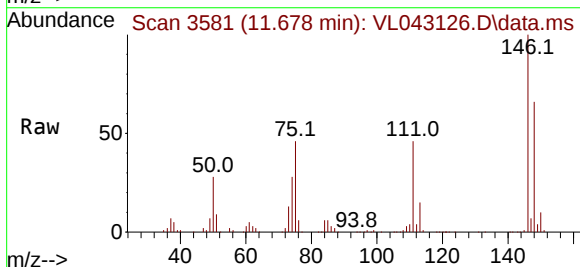



#77
 1,2-Dichlorobenzene
 Concen: 10.134 ppbv
 RT: 11.678 min Scan# 31
 Delta R.T. -0.272 min
 Lab File: VL043126.D
 Acq: 16 Oct 2025 10:26

Instrument :
 MSVOA_L
 ClientSampleId :
 RR-VOAS-AIRDL

Tgt Ion:146 Resp: 217615
 Ion Ratio Lower Upper
 146 100
 111 46.5 24.0 72.0
 148 65.4 31.1 93.3

