
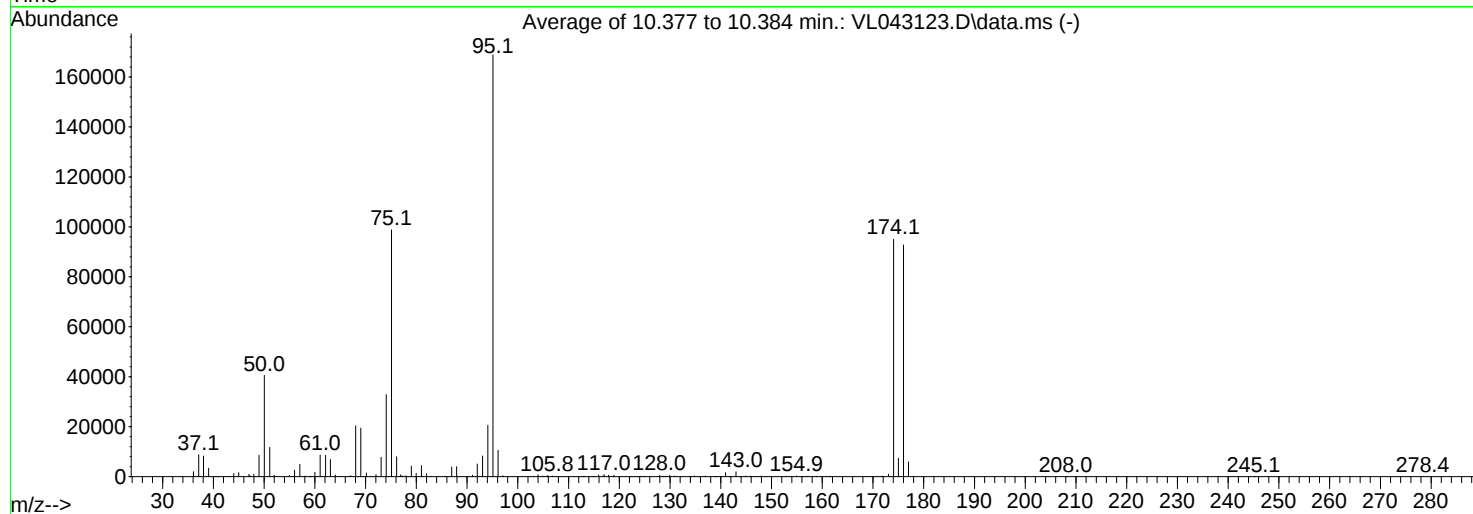


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101625\
Data File : VL043123.D
Acq On : 16 Oct 2025 08:29
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 15 02:12:58 2025

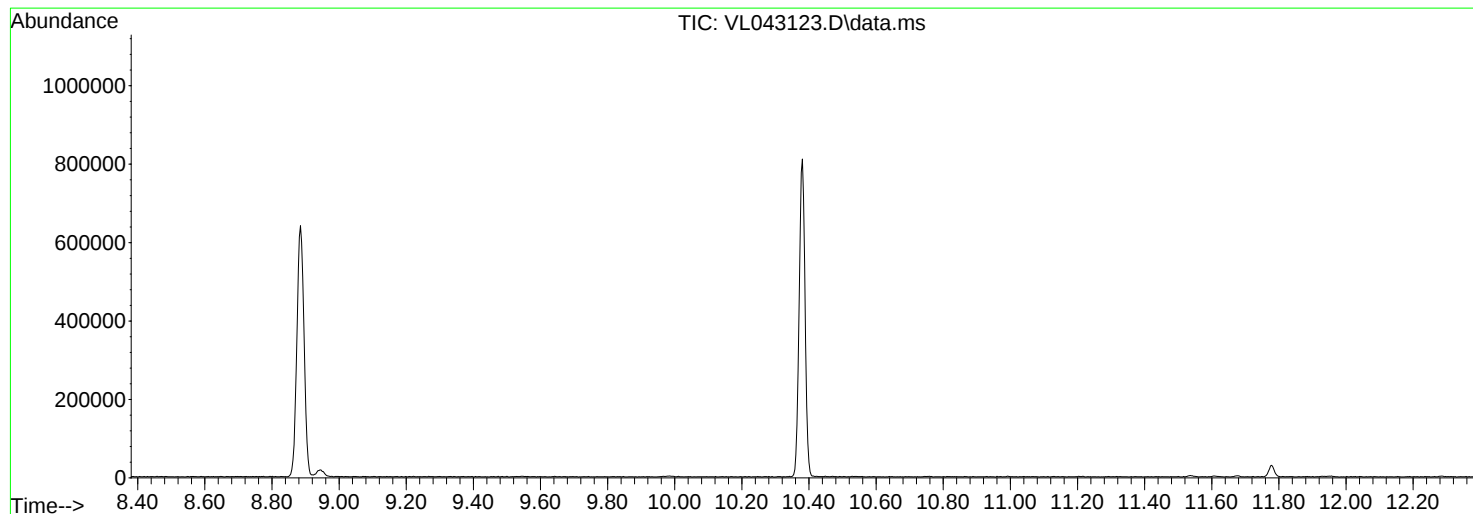

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.0	40533	PASS
75	95	30	66	58.5	98797	PASS
95	95	100	100	100.0	168853	PASS
96	95	5	9	6.3	10566	PASS
173	174	0.00	2	1.0	965	PASS
174	95	50	120	56.3	95000	PASS
175	174	4	9	7.7	7351	PASS
176	174	93	101	97.6	92741	PASS
177	176	5	9	6.4	5891	PASS

Average of 10.377 to 10.384 min.: VL043123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.80	51	46.00	143	58.05	238	69.05	1942
36.05	1979	47.00	984	59.00	24	70.15	151
37.10	8781	47.20	380	60.00	1735	70.90	11
38.05	8292	47.95	974	61.05	8626	72.05	83
39.05	3385	49.00	8510	62.10	8553	73.05	7768
39.95	3	50.05	40533	63.05	6858	74.05	32885
40.90	22	51.10	11731	64.05	616	75.10	98797
42.05	47	51.95	558	65.00	160	76.10	7925
43.00	130	54.95	485	66.80	117	76.90	728
44.00	1201	56.00	2580	67.10	382	77.20	321
45.00	1580	57.05	4916	68.05	20360	77.90	357

Average of 10.377 to 10.384 min.: VL043123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	138	93.05	8255	109.95	111	118.80	193
79.00	4211	94.10	20544	110.95	86	118.95	540
79.95	1320	95.10	168853	111.90	151	122.10	18
81.00	4417	96.10	10566	112.60	90	122.85	54
82.00	1178	97.05	366	112.90	28	123.60	32
82.90	63	103.00	54	114.80	36	124.10	191
85.70	135	104.00	797	115.05	117	124.90	22
86.95	3905	104.95	290	115.90	654	125.95	147
87.95	3946	105.80	404	116.80	321	127.95	542
91.05	558	106.00	236	117.00	812	128.70	128
92.00	5064	106.85	252	117.85	587	129.15	206

Average of 10.377 to 10.384 min.: VL043123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.90	482	143.00	1940	156.00	29	171.40	60
130.95	292	143.90	128	156.75	161	171.80	195
134.00	17	144.95	234	157.00	100	172.10	47
134.80	316	145.90	246	157.20	56	173.05	965
136.70	55	146.95	66	158.85	123	174.05	95000
136.95	225	147.95	289	160.80	202	175.00	7351
138.90	21	149.00	70	161.40	28	176.00	92741
139.85	112	150.05	160	168.80	58	177.00	5891
140.95	1579	152.85	116	169.80	26	177.90	187
141.70	66	153.80	82	170.25	52	208.00	27
142.10	148	154.95	233	170.75	43	245.10	18

Average of 10.377 to 10.384 min.: VL043123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
278.40	46						

Instrument :

MSVOA_L

ClientSampleId :

BFB