

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101722\
 Data File : VL039730.D
 Acq On : 17 Oct 2022 21:56
 Operator : SY/AP
 Sample : N5169-04 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV4

Quant Time: Oct 18 05:30:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Oct 18 05:23:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.230	49	1191284	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.687	114	3076189	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.497	117	2709100	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.802	95	1996409	9.872	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.700%
Target Compounds						
					Qvalue	
3) Chlorodifluoromethane	2.716	51	5172	0.037	ppbv	98
4) Chloromethane	2.851	50	3203	0.038	ppbv	94
9) Propene	2.735	41	67449	1.045	ppbv	92
10) Heptane	7.610	43	42457	0.282	ppbv	88
11) Trichlorofluoromethane	3.597	101	5346	0.031	ppbv	98
13) Ethanol	3.282	45	2688	0.546	ppbv #	1
15) Acetone	3.517	43	311848	2.353	ppbv	96
16) 1,3-Butadiene	3.005	39	22798	0.339	ppbv #	27
20) Methylene Chloride	3.976	84	92188	1.504	ppbv	90
23) Vinyl Acetate	4.674	43	2483	0.041	ppbv #	82
25) Ethyl Acetate	5.253	43	90357	0.313	ppbv #	79
26) Hexane	5.253	57	123372	1.006	ppbv #	40
27) Carbon Disulfide	4.166	76	52095	0.404	ppbv #	80
29) Chloroform	5.311	83	20131	0.114	ppbv #	67
30) Cyclohexane	6.639	84	43724	0.460	ppbv #	88
32) 1,1,1-Trichloroethane	6.044	97	9718	0.061	ppbv #	83
34) 2-Butanone	4.841	43	39434	0.261	ppbv	92
35) Carbon Tetrachloride	6.533	117	197563	1.210	ppbv	93
38) Trichloroethene	7.324	130	166934	1.313	ppbv	100
39) 1,2-Dichloropropane	6.687	63	765173	8.426	ppbv #	25
44) 2,2,4-Trimethylpentane	7.362	57	23025	0.057	ppbv #	15
52) Tetrachloroethene	10.645	164	2715	0.030	ppbv #	42
53) Toluene	9.253	91	404278	1.546	ppbv	98
58) Ethyl Benzene	12.121	91	65474	0.210	ppbv	97
59) m/p-Xylene	12.372	91	531072	1.910	ppbv	99
60) o-Xylene	13.089	91	171369	0.646	ppbv	98
64) n-propylbenzene	14.950	120	5832	0.057	ppbv #	1
70) n-Butylbenzene	17.921	91	17769	0.045	ppbv #	17
71) 2-Chlorotoluene	14.703	91	23388	0.081	ppbv #	44
72) 4-Ethyltoluene	15.227	105	55310	0.183	ppbv #	48
73) 1,3,5-Trimethylbenzene	15.375	105	84527	0.305	ppbv	86
74) 1,2,4-Trimethylbenzene	16.137	105	436654	1.405	ppbv #	70
79) Naphthalene	21.407	128	7123	0.035	ppbv	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101722\
Data File : VL039730.D
Acq On : 17 Oct 2022 21:56
Operator : SY/AP
Sample : N5169-04 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV4

Quant Time: Oct 18 05:30:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Oct 18 05:23:57 2022
Response via : Initial Calibration




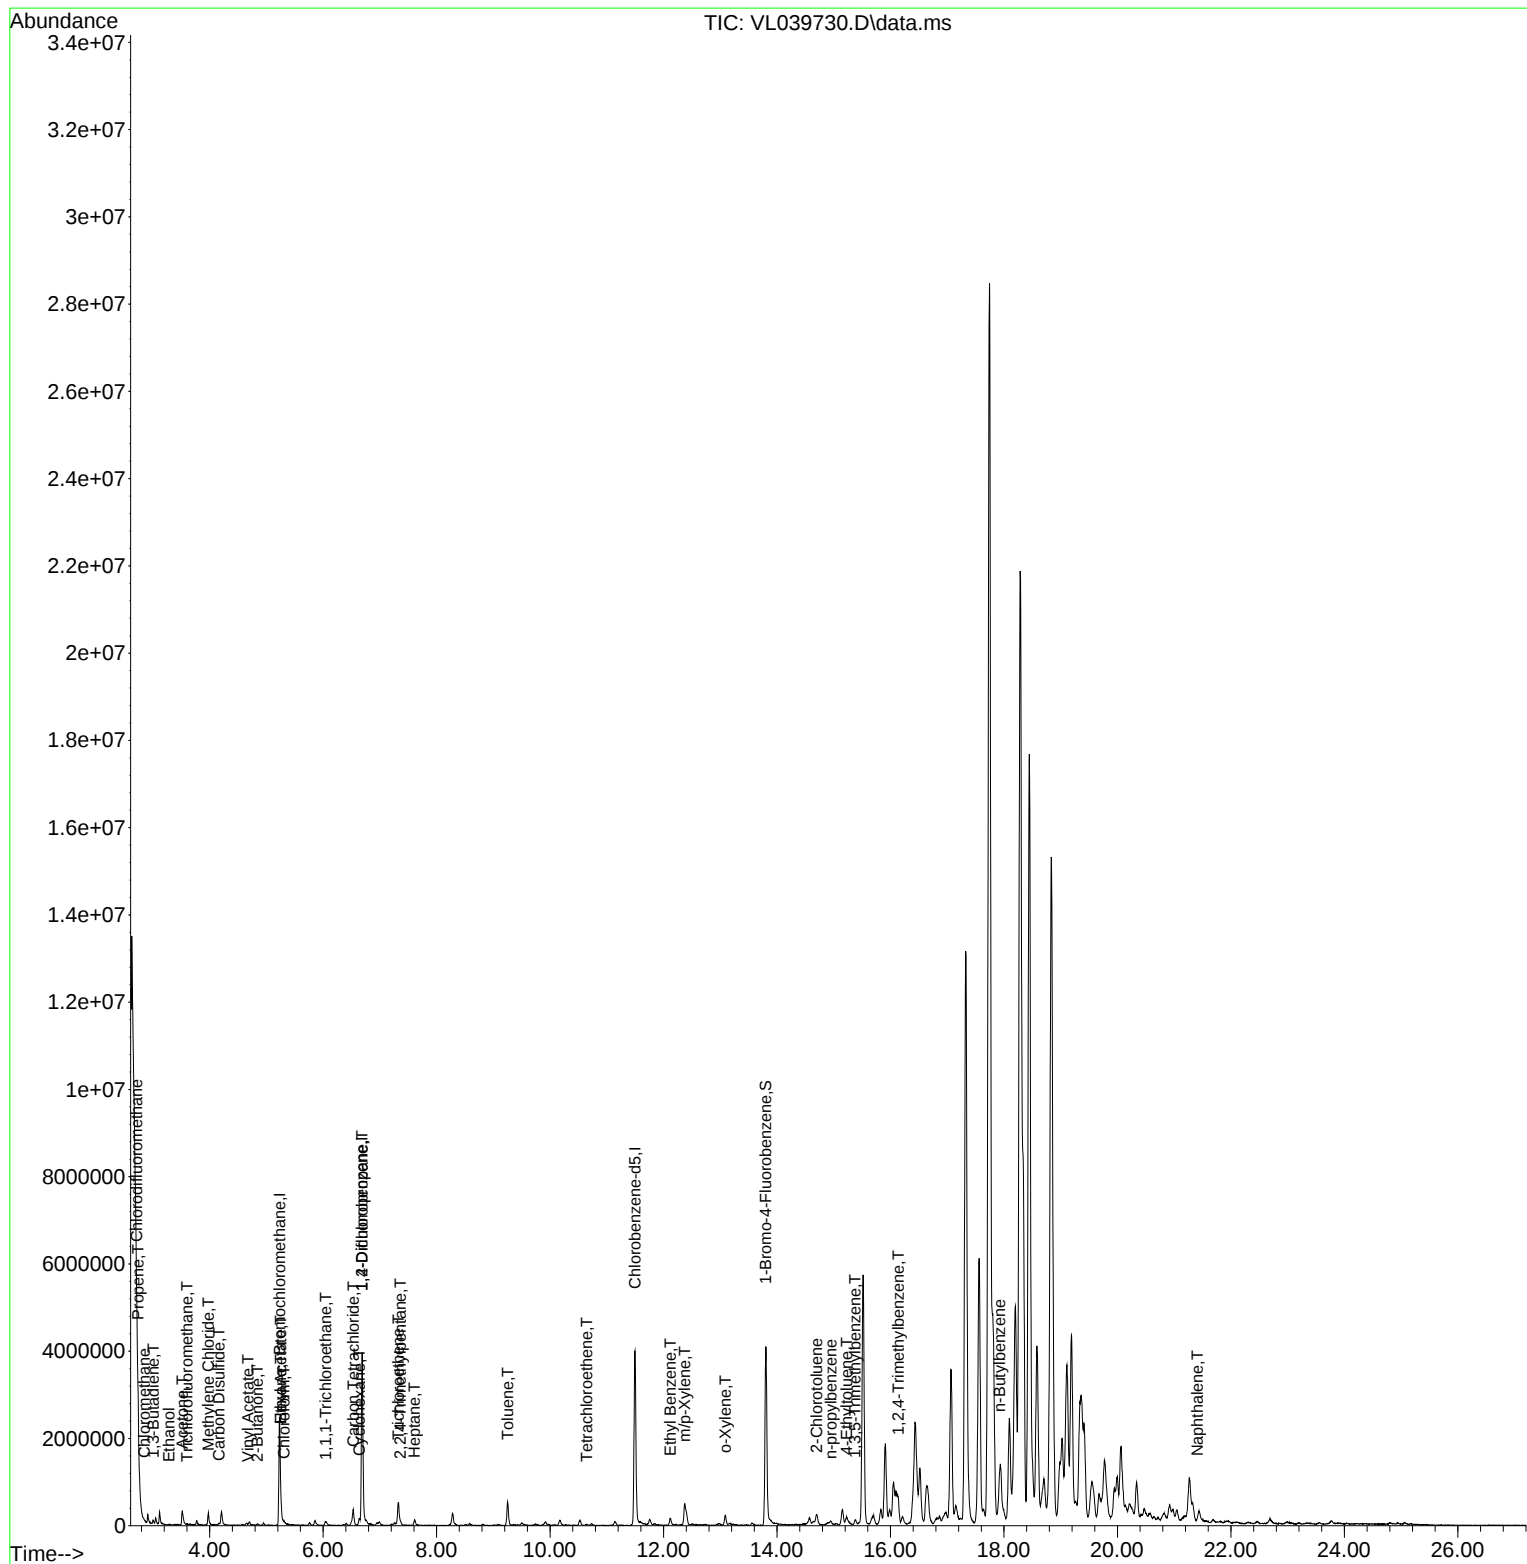




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.230 min Scan# 81
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 49 Resp: 1191284
Ion Ratio Lower Upper
49 100
128 48.0 26.7 80.0
130 61.3 34.3 102.8

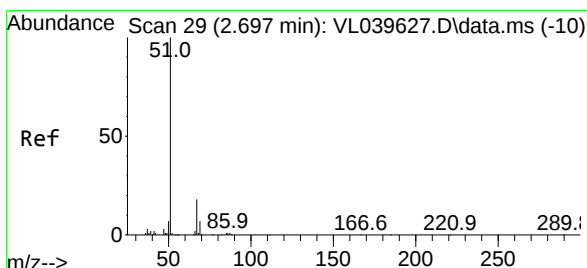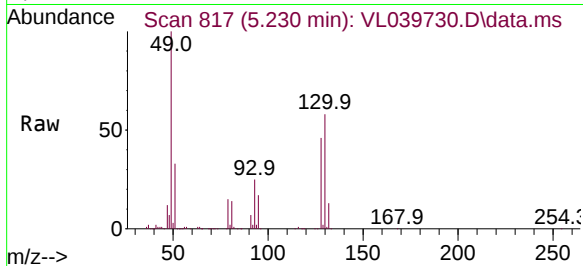

#3
Chlorodifluoromethane
Concen: 0.037 ppbv
RT: 2.716 min Scan# 35
Delta R.T. 0.003 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 51 Resp: 5172
Ion Ratio Lower Upper
51 100
67 20.6 15.7 23.5

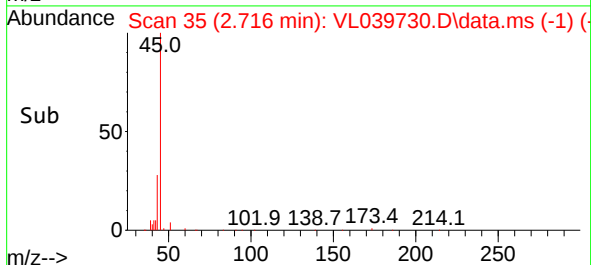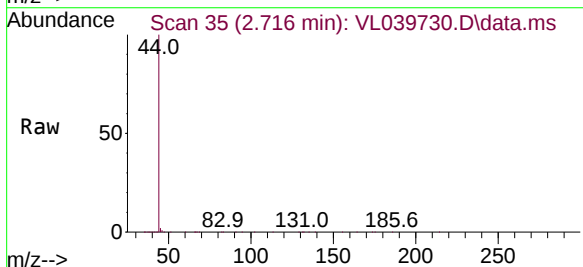

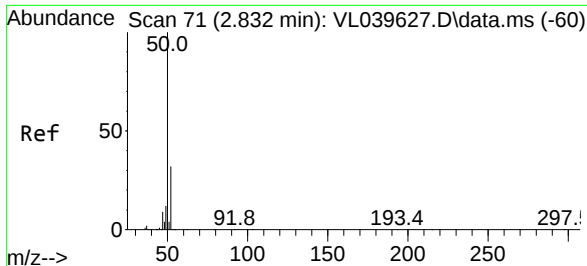

#4
Chloromethane
Concen: 0.038 ppbv
RT: 2.851 min Scan# 71
Delta R.T. -0.000 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56





Instrument :

MSVOA_L

ClientSampleId :




SV4


Tgt Ion: 50 Resp: 3203
Ion Ratio Lower Upper
50 100
52 29.5 26.5 39.7

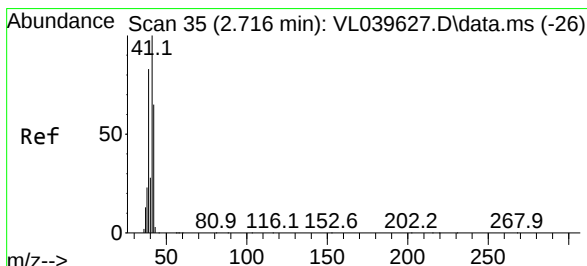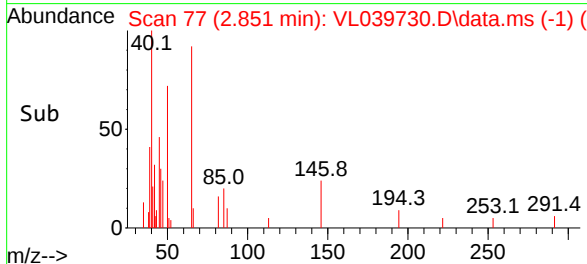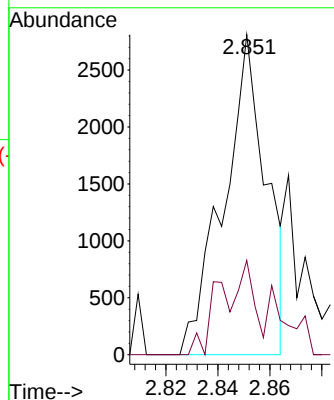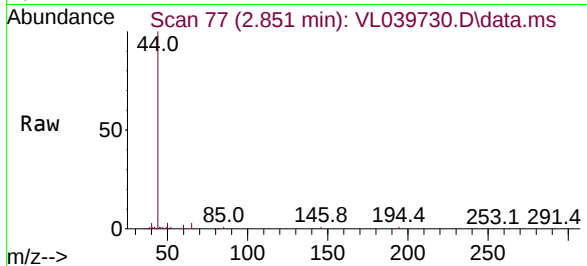

#9
Propene
Concen: 1.045 ppbv
RT: 2.735 min Scan# 41
Delta R.T. 0.003 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 41 Resp: 67449
Ion Ratio Lower Upper
41 100
42 75.8 55.2 82.8


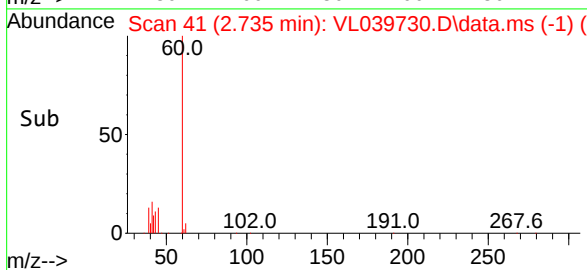
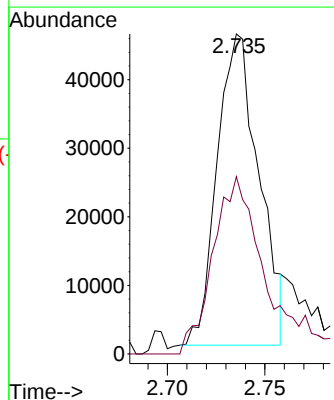
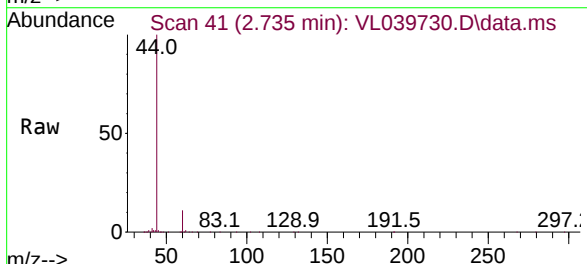




#10
Heptane
Concen: 0.282 ppbv
RT: 7.610 min Scan# 11
Delta R.T. -0.000 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 43 Resp: 42457
Ion Ratio Lower Upper
43 100
57 59.0 40.5 60.7

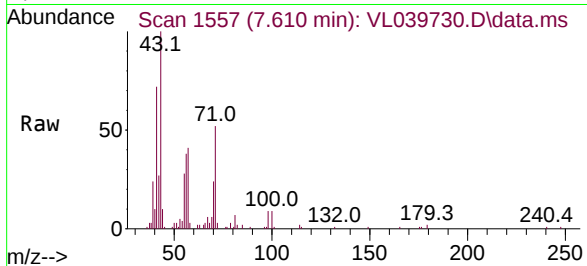

#11
Trichlorofluoromethane
Concen: 0.031 ppbv
RT: 3.597 min Scan# 309
Delta R.T. -0.003 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 101 Resp: 5346
Ion Ratio Lower Upper
101 100
103 66.4 51.8 77.8


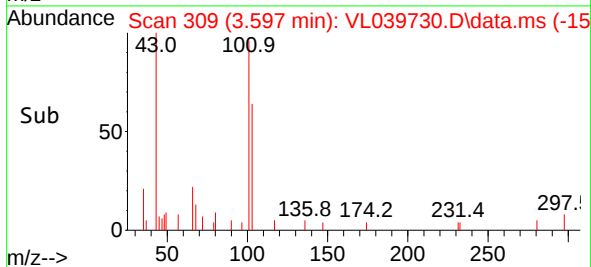

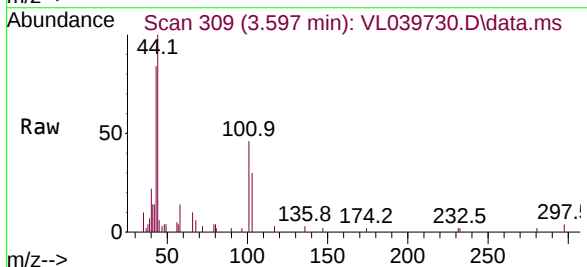




#13
Ethanol
Concen: 0.546 ppbv
RT: 3.282 min Scan# 211
Delta R.T. -0.000 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 45 Resp: 2688
Ion Ratio Lower Upper
45 100
46 159.6 22.8 91.2#

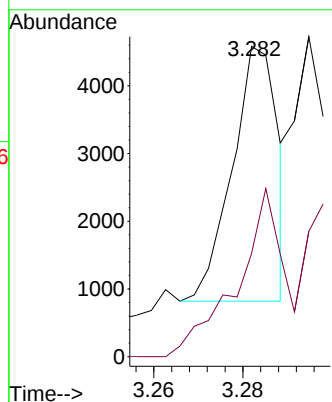

#15
Acetone
Concen: 2.353 ppbv
RT: 3.517 min Scan# 284
Delta R.T. 0.013 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 43 Resp: 311848
Ion Ratio Lower Upper
43 100
58 28.5 21.0 31.6


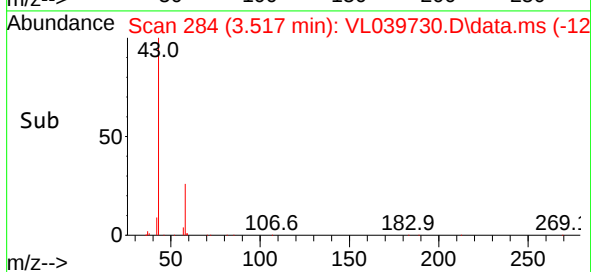
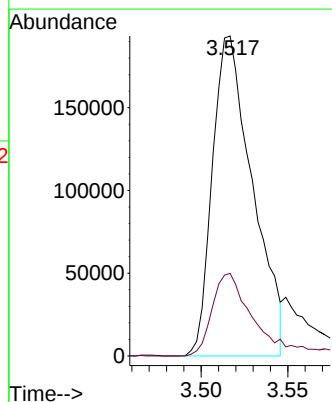





#16
1,3-Butadiene
Concen: 0.339 ppbv
RT: 3.005 min Scan# 11
Delta R.T. -0.016 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 39 Resp: 22798
Ion Ratio Lower Upper
39 100
54 15.3 63.7 95.5#

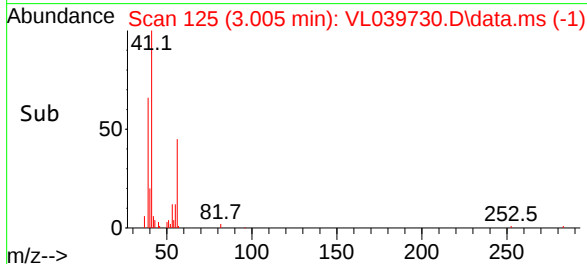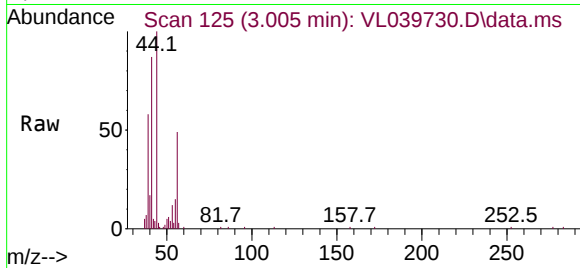

#20
Methylene Chloride
Concen: 1.504 ppbv
RT: 3.976 min Scan# 427
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 84 Resp: 92188
Ion Ratio Lower Upper
84 100
49 166.0 123.1 184.7
51 51.1 34.4 51.6
86 71.8 51.1 76.7




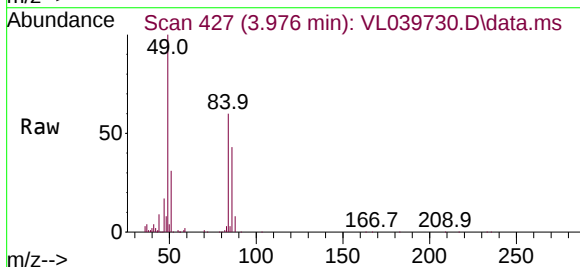




#23
 Vinyl Acetate
 Concen: 0.041 ppbv
 RT: 4.674 min Scan# 644
 Delta R.T. 0.013 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56




Instrument :
 MSVOA_L
 ClientSampleId :
 SV4


Tgt Ion:	43	Resp:	2483
Ion	Ratio	Lower	Upper
43	100		
86	4.9	5.0	7.6#
42	0.0	7.7	11.5#
44	12.1	4.6	7.0#

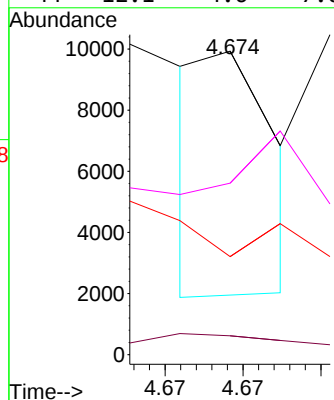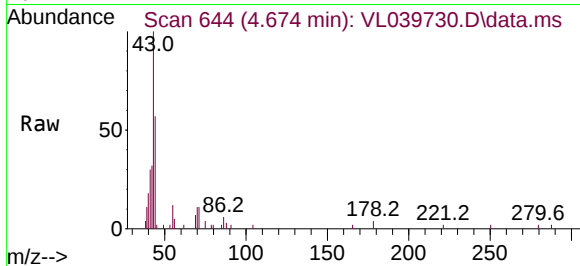

#25
 Ethyl Acetate
 Concen: 0.313 ppbv
 RT: 5.253 min Scan# 824
 Delta R.T. 0.013 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56

Tgt Ion:	43	Resp:	90357
Ion	Ratio	Lower	Upper
43	100		
45	2.8	8.2	12.4#
61	0.4	8.3	12.5#
70	2.4	5.9	8.9#



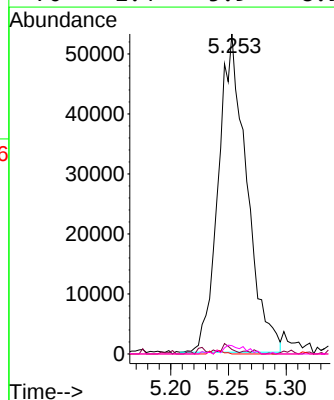
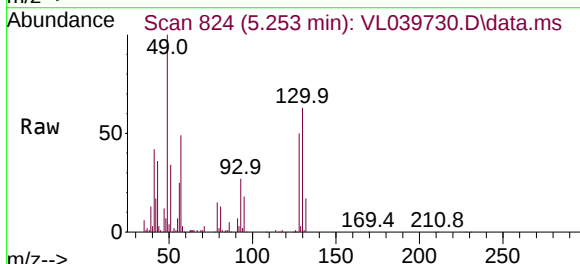




#26
Hexane
Concen: 1.006 ppbv
RT: 5.253 min Scan# 816
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 57 Resp: 123372
Ion Ratio Lower Upper
57 100
41 98.3 76.9 115.3
43 76.8 191.0 286.6#
56 58.5 43.2 64.8

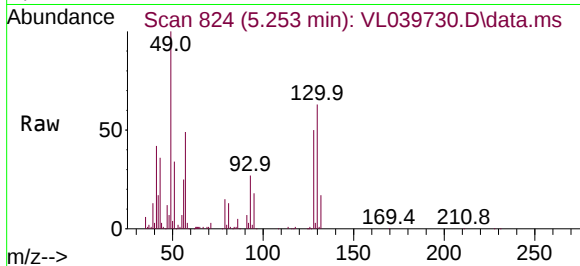

#27
Carbon Disulfide
Concen: 0.404 ppbv
RT: 4.166 min Scan# 486
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 76 Resp: 52095
Ion Ratio Lower Upper
76 100
44 30.3 14.6 21.8#
78 12.0 7.8 11.6#

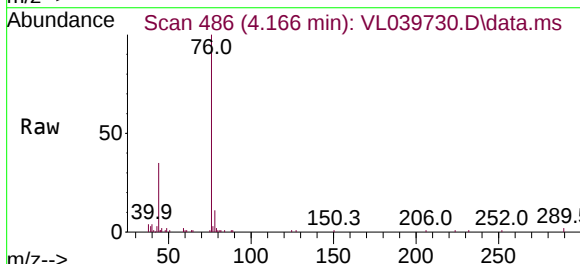



#29

Chloroform

Concen: 0.114 ppbv

RT: 5.311 min Scan# 84

Delta R.T. 0.003 min

Lab File: VL039730.D

Acq: 17 Oct 2022 21:56

Instrument :

MSVOA_L

ClientSampleId :





SV4

Tgt Ion: 83 Resp: 20131

Ion Ratio Lower Upper

83 100

85 39.7 52.8 79.2#

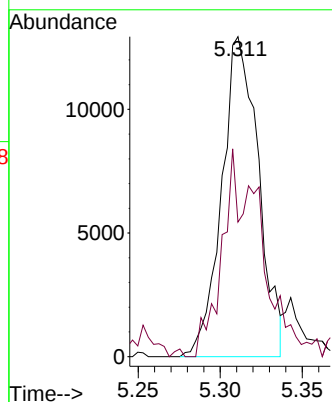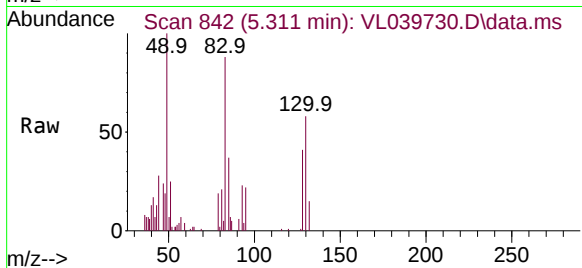

#30

Cyclohexane

Concen: 0.460 ppbv

RT: 6.639 min Scan# 1255

Delta R.T. 0.006 min

Lab File: VL039730.D

Acq: 17 Oct 2022 21:56




Tgt Ion: 84 Resp: 43724


Ion Ratio Lower Upper

84 100

56 129.0 107.7 161.5

41 105.0 67.7 101.5#




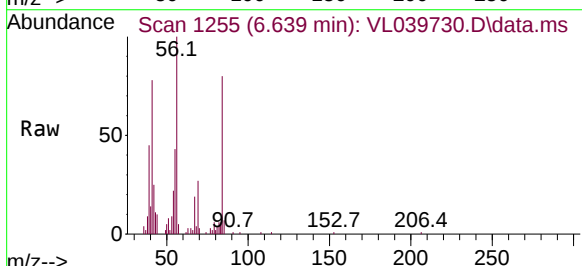




#32
 1,1,1-Trichloroethane
 Concen: 0.061 ppbv
 RT: 6.044 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56




Instrument :
 MSVOA_L
 ClientSampleId :
 SV4


Tgt Ion: 97 Resp: 9718
 Ion Ratio Lower Upper
 97 100
 99 74.5 52.3 78.5
 61 68.1 40.9 61.3#

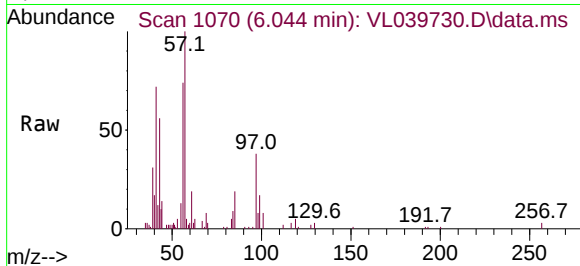

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 6.687 min Scan# 1270
 Delta R.T. -0.000 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56

Tgt Ion: 114 Resp: 3076189
 Ion Ratio Lower Upper
 114 100
 63 25.4 20.2 30.4
 88 18.3 14.5 21.7




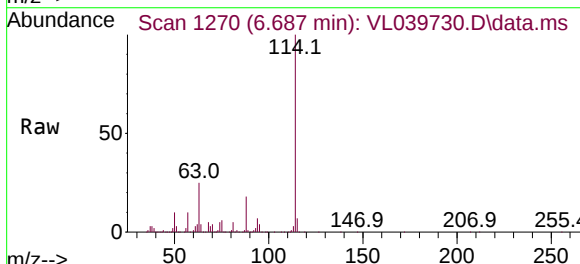




#34
2-Butanone
Concen: 0.261 ppbv
RT: 4.841 min Scan# 61
Delta R.T. 0.019 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 43 Resp: 39434
Ion Ratio Lower Upper
43 100
72 26.4 17.9 26.9

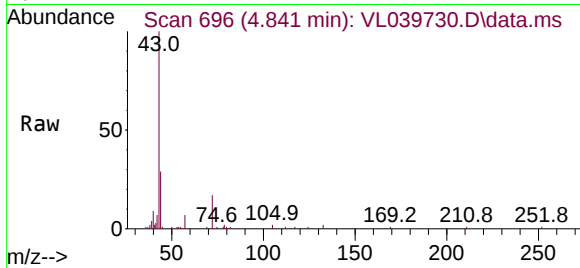

#35
Carbon Tetrachloride
Concen: 1.210 ppbv
RT: 6.533 min Scan# 1222
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 117 Resp: 197563
Ion Ratio Lower Upper
117 100
119 86.4 75.4 113.2
121 32.2 24.2 36.2


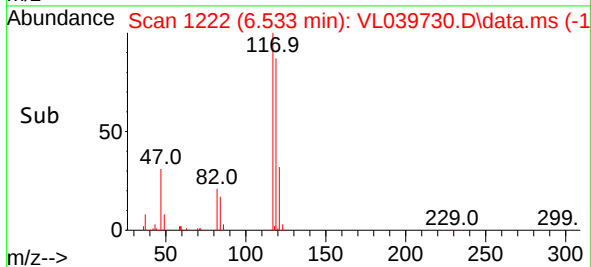

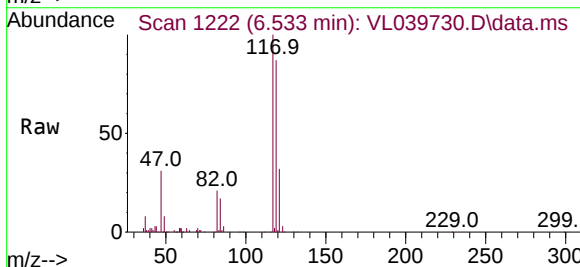




#38
 Trichloroethene
 Concen: 1.313 ppbv
 RT: 7.324 min Scan# 1461
 Delta R.T. -0.000 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56




Instrument :
 MSVOA_L
 ClientSampleId :
 SV4


Tgt Ion:	130	Resp:	166934
Ion	Ratio	Lower	Upper
130	100		
95	109.6	87.3	130.9
132	95.9	76.7	115.1
97	70.5	56.5	84.7

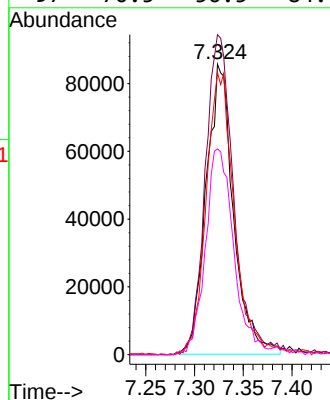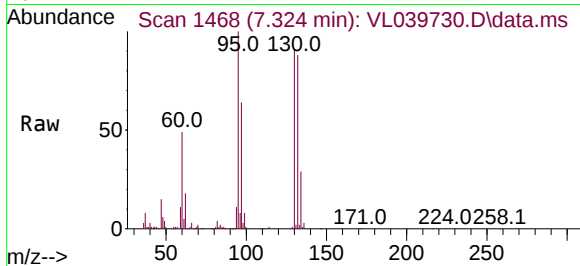

#39
 1,2-Dichloropropane
 Concen: 8.426 ppbv
 RT: 6.687 min Scan# 1270
 Delta R.T. -0.418 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56

Tgt Ion:	63	Resp:	765173
Ion	Ratio	Lower	Upper
63	100		
41	0.0	59.6	89.4#
62	16.8	51.4	77.0#

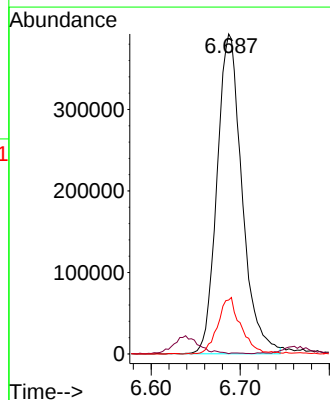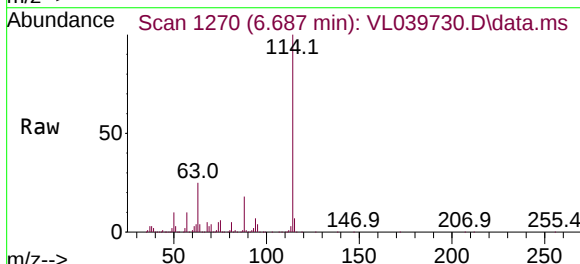



#44

2,2,4-Trimethylpentane

Concen: 0.057 ppbv

RT: 7.362 min Scan# 14

Delta R.T. 0.006 min

Lab File: VL039730.D

Acq: 17 Oct 2022 21:56

Instrument :

MSVOA_L

ClientSampleId :

SV4





Tgt Ion: 57 Resp: 23025

Ion Ratio Lower Upper

57 100

41 98.5 27.4 41.2#

56 0.0 24.5 36.7#

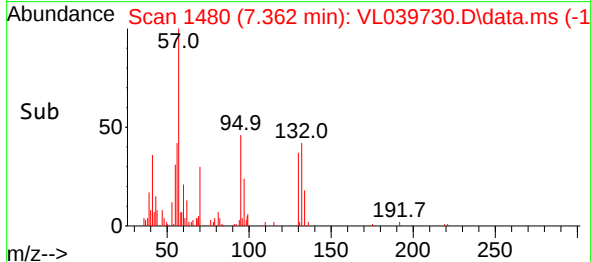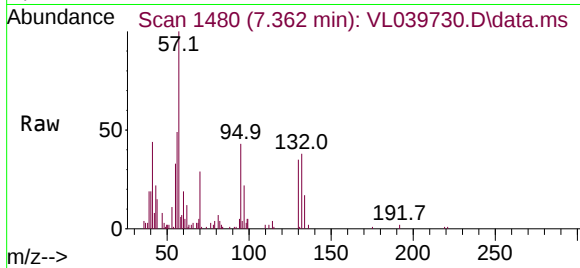

#52

Tetrachloroethene

Concen: 0.030 ppbv

RT: 10.645 min Scan# 2501

Delta R.T. -0.000 min

Lab File: VL039730.D

Acq: 17 Oct 2022 21:56

Tgt Ion: 164 Resp: 2715




Ion Ratio Lower Upper


164 100

166 95.7 102.2 153.2#

129 8.9 85.8 128.8#

131 46.6 83.3 124.9#


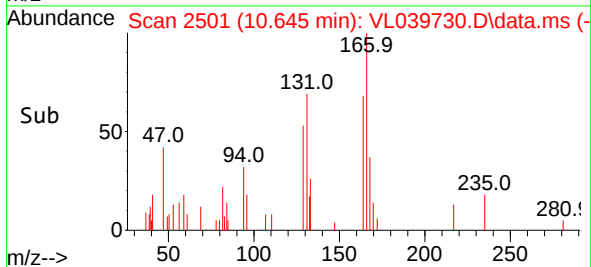

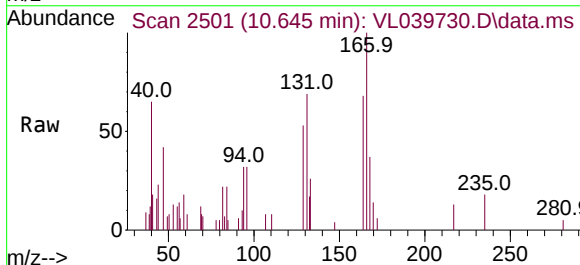




#53
Toluene
Concen: 1.546 ppbv
RT: 9.253 min Scan# 2060
Delta R.T. 0.003 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 404278
Ion Ratio Lower Upper
91 100
92 58.8 48.2 72.2

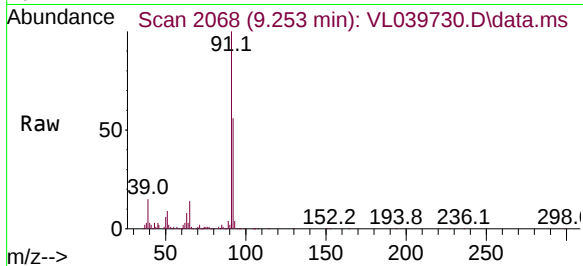

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.497 min Scan# 2766
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 117 Resp: 2709100
Ion Ratio Lower Upper
117 100
82 63.7 50.8 76.2
119 33.4 24.1 36.1




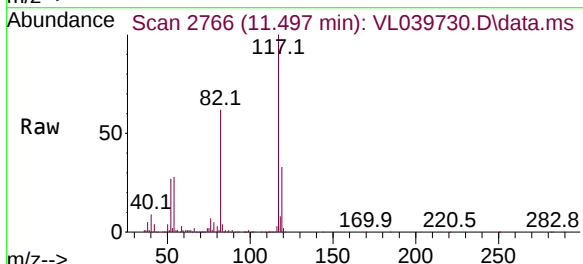




#58
Ethyl Benzene
Concen: 0.210 ppbv
RT: 12.121 min Scan# 2953
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 65474
Ion Ratio Lower Upper
91 100
106 29.9 25.4 38.0

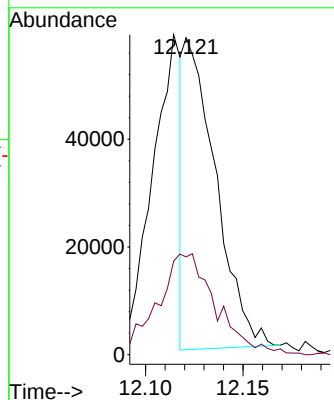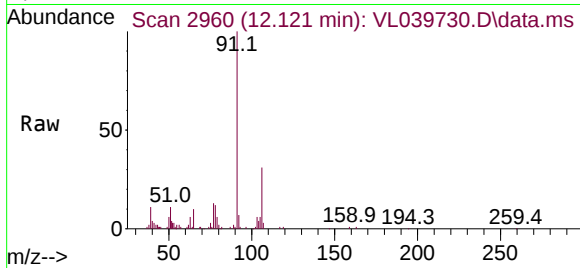

#59
m/p-Xylene
Concen: 1.910 ppbv
RT: 12.372 min Scan# 3038
Delta R.T. -0.029 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 91 Resp: 531072
Ion Ratio Lower Upper
91 100
106 45.3 35.4 53.2



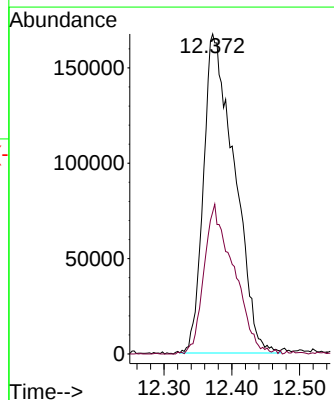
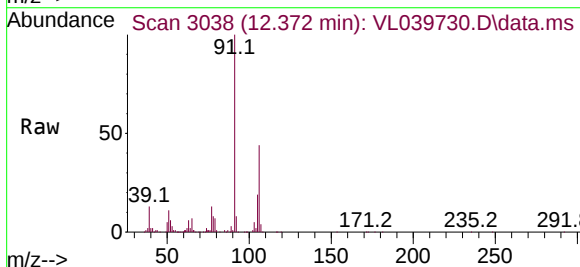




#60
o-Xylene
Concen: 0.646 ppbv
RT: 13.089 min Scan# 31
Delta R.T. 0.003 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 171369
Ion Ratio Lower Upper
91 100
106 46.1 22.4 67.3

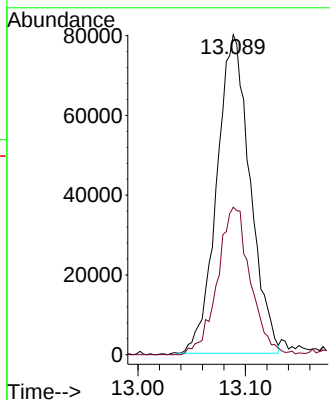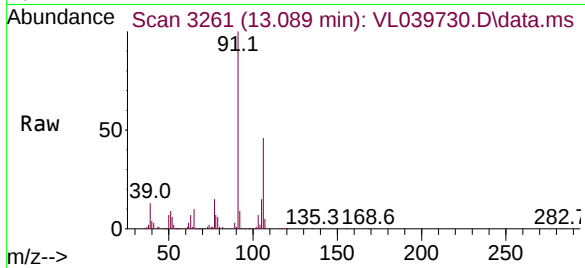

#64
n-propylbenzene
Concen: 0.057 ppbv
RT: 14.950 min Scan# 3840
Delta R.T. 0.010 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 120 Resp: 5832
Ion Ratio Lower Upper
120 100
91 1537.4 367.2 550.8#



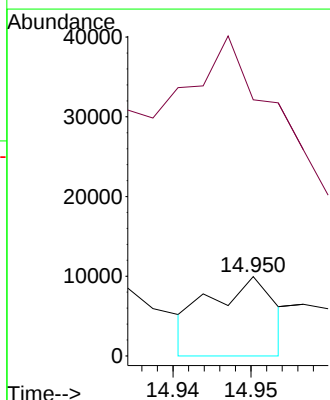
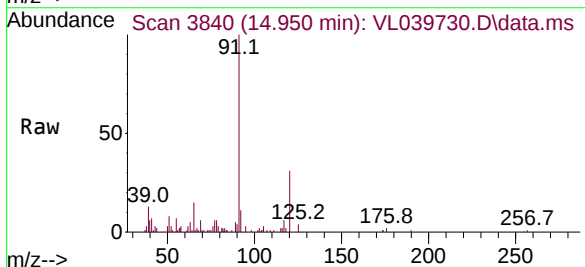




#68
1-Bromo-4-Fluorobenzene
Concen: 9.872 ppbv
RT: 13.802 min Scan# 3476
Delta R.T. 0.003 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 95 Resp: 1996409
Ion Ratio Lower Upper
95 100
174 71.8 55.9 83.9
175 5.2 4.2 6.4

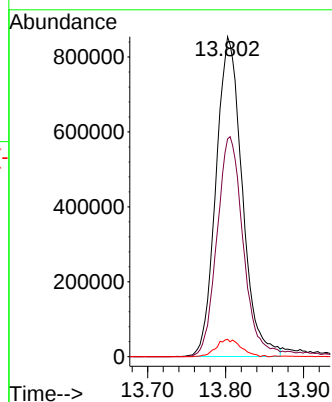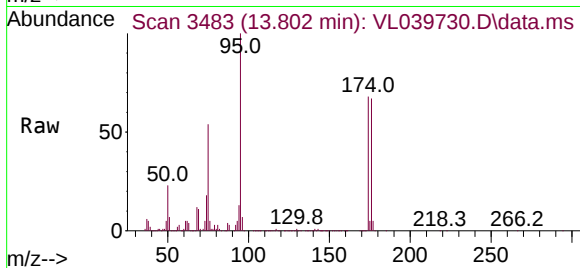

#70
n-Butylbenzene
Concen: 0.045 ppbv
RT: 17.921 min Scan# 4764
Delta R.T. 0.010 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 91 Resp: 17769
Ion Ratio Lower Upper
91 100
92 124.6 43.4 65.2#
134 0.0 18.9 28.3#


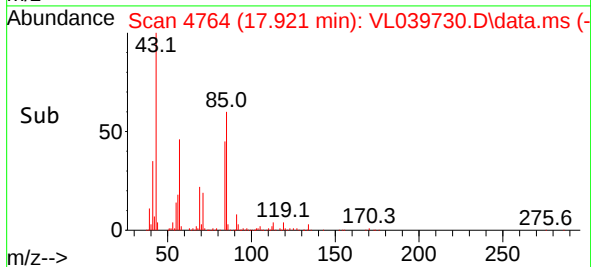

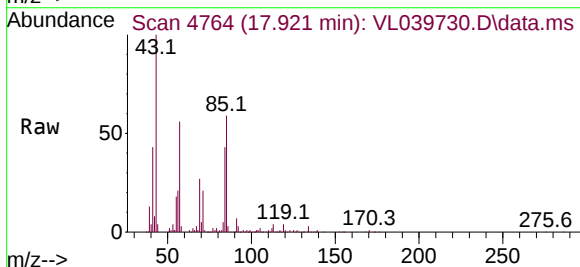




#71
2-Chlorotoluene
Concen: 0.081 ppbv
RT: 14.703 min Scan# 31
Delta R.T. -0.125 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56




Instrument :
MSVOA_L
ClientSampleId :
SV4


Tgt Ion: 91 Resp: 23388
Ion Ratio Lower Upper
91 100
126 1.0 13.0 51.8#

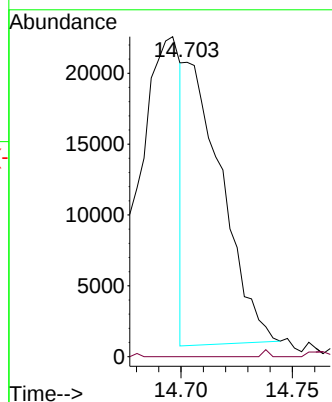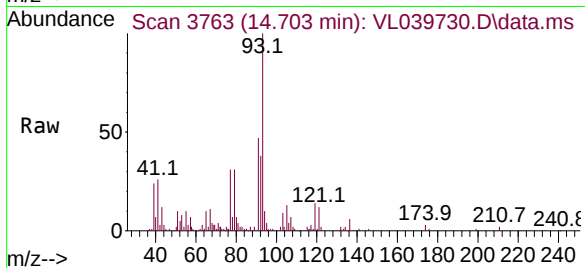

#72
4-Ethyltoluene
Concen: 0.183 ppbv
RT: 15.227 min Scan# 3926
Delta R.T. 0.006 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Tgt Ion: 105 Resp: 55310
Ion Ratio Lower Upper
105 100
120 64.1 24.2 36.2#
91 24.3 10.2 15.4#
77 35.3 11.1 16.7#




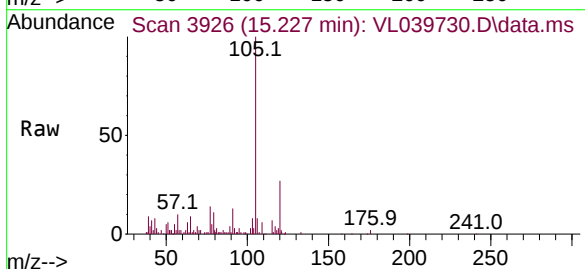


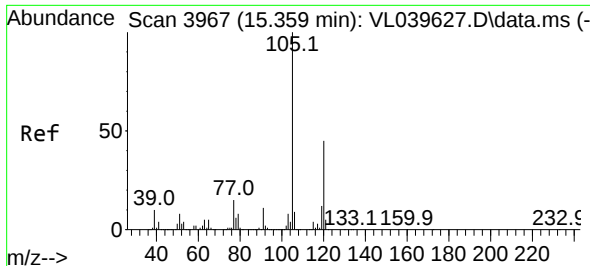

#73
 1,3,5-Trimethylbenzene
 Concen: 0.305 ppbv
 RT: 15.375 min Scan# 3967
 Delta R.T. -0.003 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56




Instrument :
 MSVOA_L
 ClientSampleId :
 SV4


Tgt Ion:105 Resp: 84527
 Ion Ratio Lower Upper
 105 100
 120 38.6 38.2 57.4

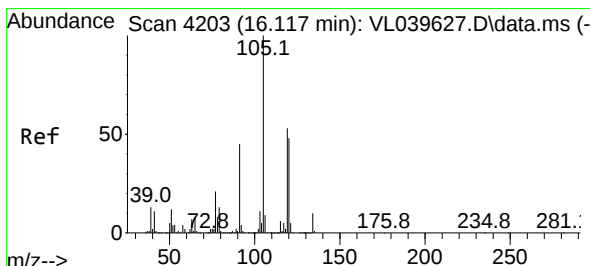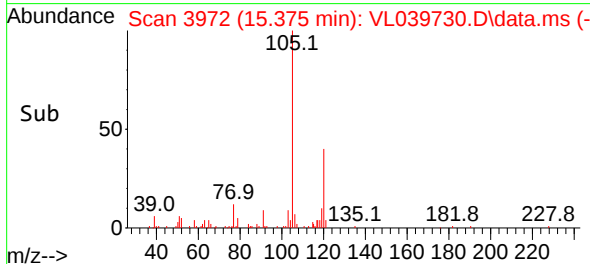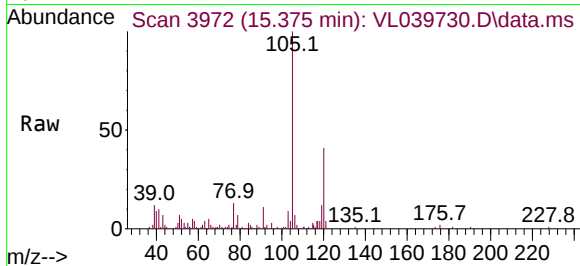

#74
 1,2,4-Trimethylbenzene
 Concen: 1.405 ppbv
 RT: 16.137 min Scan# 4209
 Delta R.T. 0.003 min
 Lab File: VL039730.D
 Acq: 17 Oct 2022 21:56

Tgt Ion:105 Resp: 436654
 Ion Ratio Lower Upper
 105 100
 120 42.6 39.5 59.3
 91 10.6 39.2 58.8#
 77 14.2 17.2 25.8#

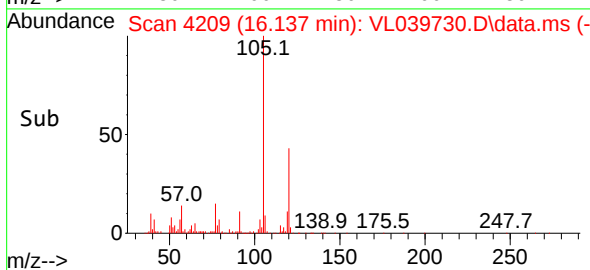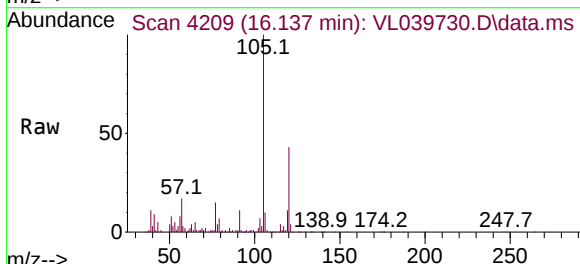



#79
Naphthalene
Concen: 0.035 ppbv
RT: 21.407 min Scan# 51
Delta R.T. -0.000 min
Lab File: VL039730.D
Acq: 17 Oct 2022 21:56

Instrument :
MSVOA_L
ClientSampleId :
SV4

Tgt Ion:128 Resp: 7123
Ion Ratio Lower Upper
128 100
127 15.8 10.6 15.8
129 12.8 8.8 13.2

