
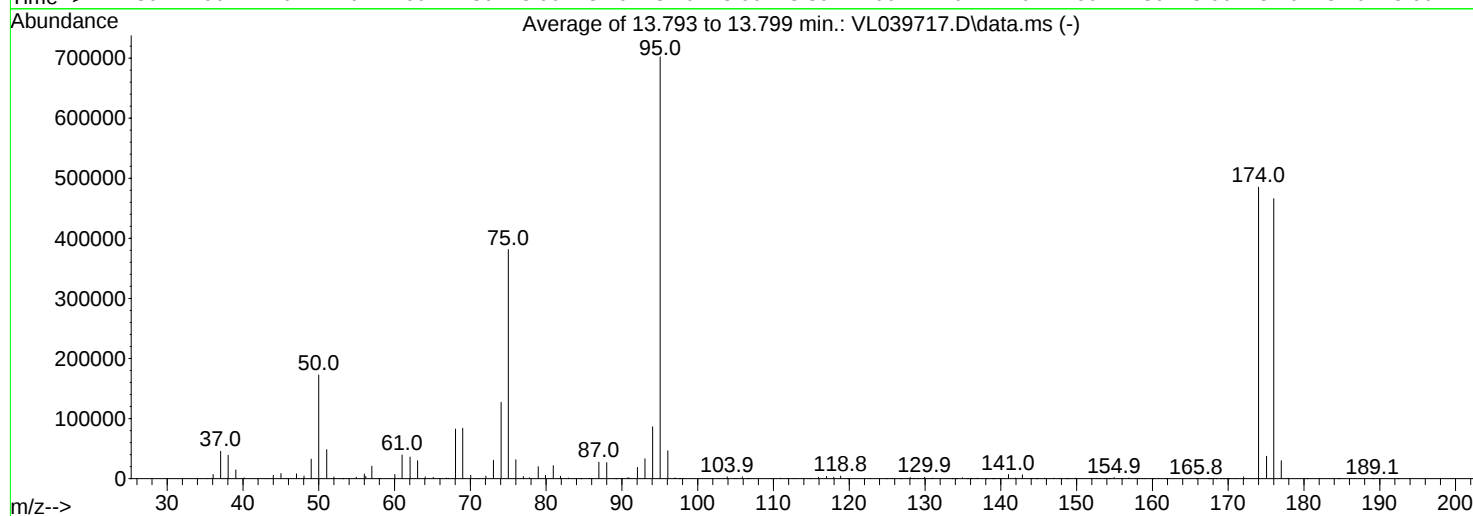


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101722\
 Data File : VL039717.D
 Acq On : 17 Oct 2022 12:32
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Oct 18 05:23:57 2022

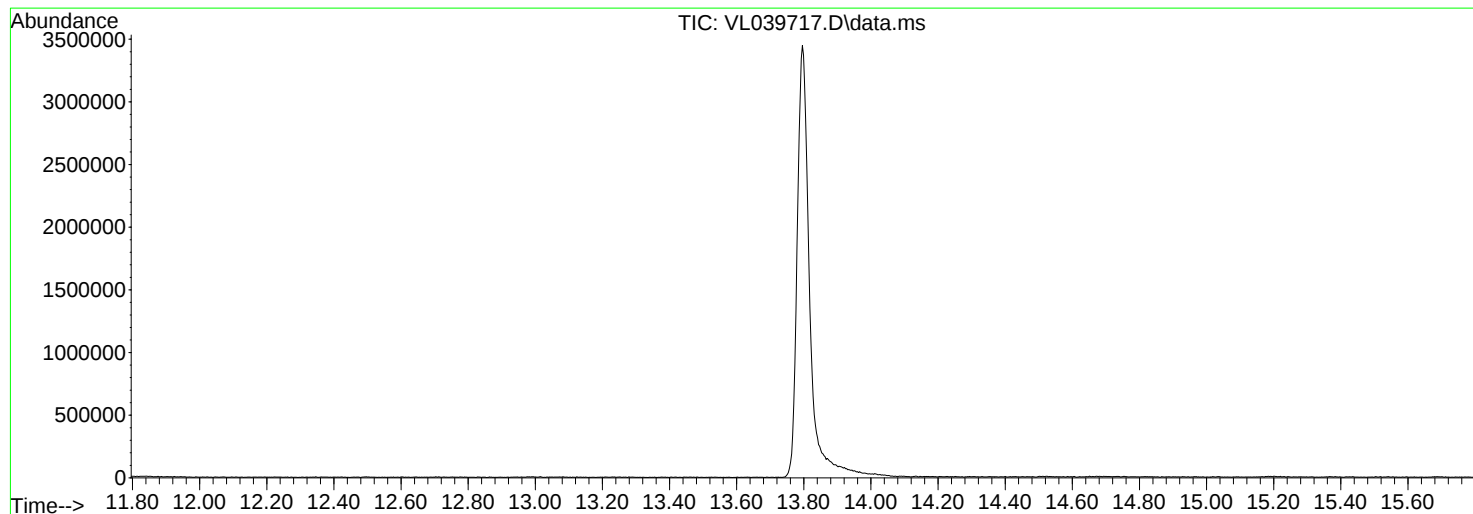

AutoFind: Scans 3480, 3481, 3482; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.6	172715	PASS
75	95	30	66	54.3	381419	PASS
95	95	100	100	100.0	702101	PASS
96	95	5	9	6.6	46307	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.1	485141	PASS
175	174	4	9	7.7	37315	PASS
176	174	93	101	96.1	466133	PASS
177	176	5	9	6.4	29869	PASS

Average of 13.793 to 13.799 min.: VL039717.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.25	248	46.00	314	56.20	3839	66.85	1211
36.05	6951	47.05	7959	57.00	20840	67.10	581
37.05	45488	48.05	4555	57.90	611	68.05	8246
38.05	39021	49.00	32592	58.10	630	69.00	8388
39.05	14535	50.00	172715	60.05	6978	70.05	5751
40.15	1472	51.05	48192	61.00	39339	70.90	330
43.00	252	52.00	2813	62.05	35840	71.20	199
43.30	226	52.80	252	63.05	29752	72.05	4260
44.00	5527	53.15	125	64.05	2869	73.05	30677
45.00	8501	54.95	2526	65.10	2286	74.05	127045
45.80	303	56.00	7819	66.35	297	75.00	381419

Average of 13.793 to 13.799 min.: VL039717.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	31531	86.05	344	96.05	46307	110.10	263
77.00	3445	86.95	27552	97.00	1354	110.95	899
77.80	1709	88.00	26582	97.60	69	111.80	280
78.95	20032	89.20	83	102.80	224	112.60	473
79.90	5683	90.10	203	103.90	2926	112.90	164
80.95	21528	90.80	1867	104.90	346	113.20	259
81.90	3907	91.00	777	105.10	617	114.90	580
82.95	1193	92.05	18569	105.90	2916	115.95	2270
83.80	357	93.05	33136	106.60	76	117.00	3761
84.60	117	94.05	86275	107.00	596	117.95	2507
85.75	488	95.05	702101	109.70	220	118.85	4241

Average of 13.793 to 13.799 min.: VL039717.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.80	57	129.10	541	138.10	92	144.95	623
120.10	229	129.95	2491	138.45	234	145.75	816
122.80	230	130.80	493	138.90	86	147.00	761
124.00	619	131.05	942	139.20	125	147.80	390
124.85	159	133.60	69	139.75	427	148.00	826
125.70	169	134.10	53	141.00	7018	148.70	147
125.95	266	134.95	1541	141.95	1001	149.00	502
126.80	87	135.60	64	142.85	6280	149.80	850
127.70	428	136.10	80	143.90	291	151.95	592
128.05	1896	136.70	307	144.10	473	152.60	169
128.65	669	136.95	861	144.70	132	153.00	666

Average of 13.793 to 13.799 min.: VL039717.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.70	618	161.80	77	172.05	2882		
154.30	127	165.80	117	174.00	485141		
154.95	1781	167.40	75	175.05	37315		
156.00	108	167.65	155	176.00	466133		
156.90	1022	168.40	59	177.00	29869		
157.80	238	169.00	96	177.90	768		
158.30	223	169.40	105	180.40	85		
158.70	258	169.80	125	184.60	81		
159.00	343	170.10	148	189.05	120		
160.10	93	170.75	370	192.40	106		
160.85	614	171.10	202				