

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101725\
 Data File : VL043132.D
 Acq On : 17 Oct 2025 09:05
 Operator : SY/MD
 Sample : VL1017ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL1017ABL01

Quant Time: Oct 18 04:32:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Oct 15 02:12:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	88811	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	284361	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	240318	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	189815	10.162	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101725\
Data File : VL043132.D
Acq On : 17 Oct 2025 09:05
Operator : SY/MD
Sample : VL1017ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL1017ABL01

Quant Time: Oct 18 04:32:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed Oct 15 02:12:58 2025
Response via : Initial Calibration




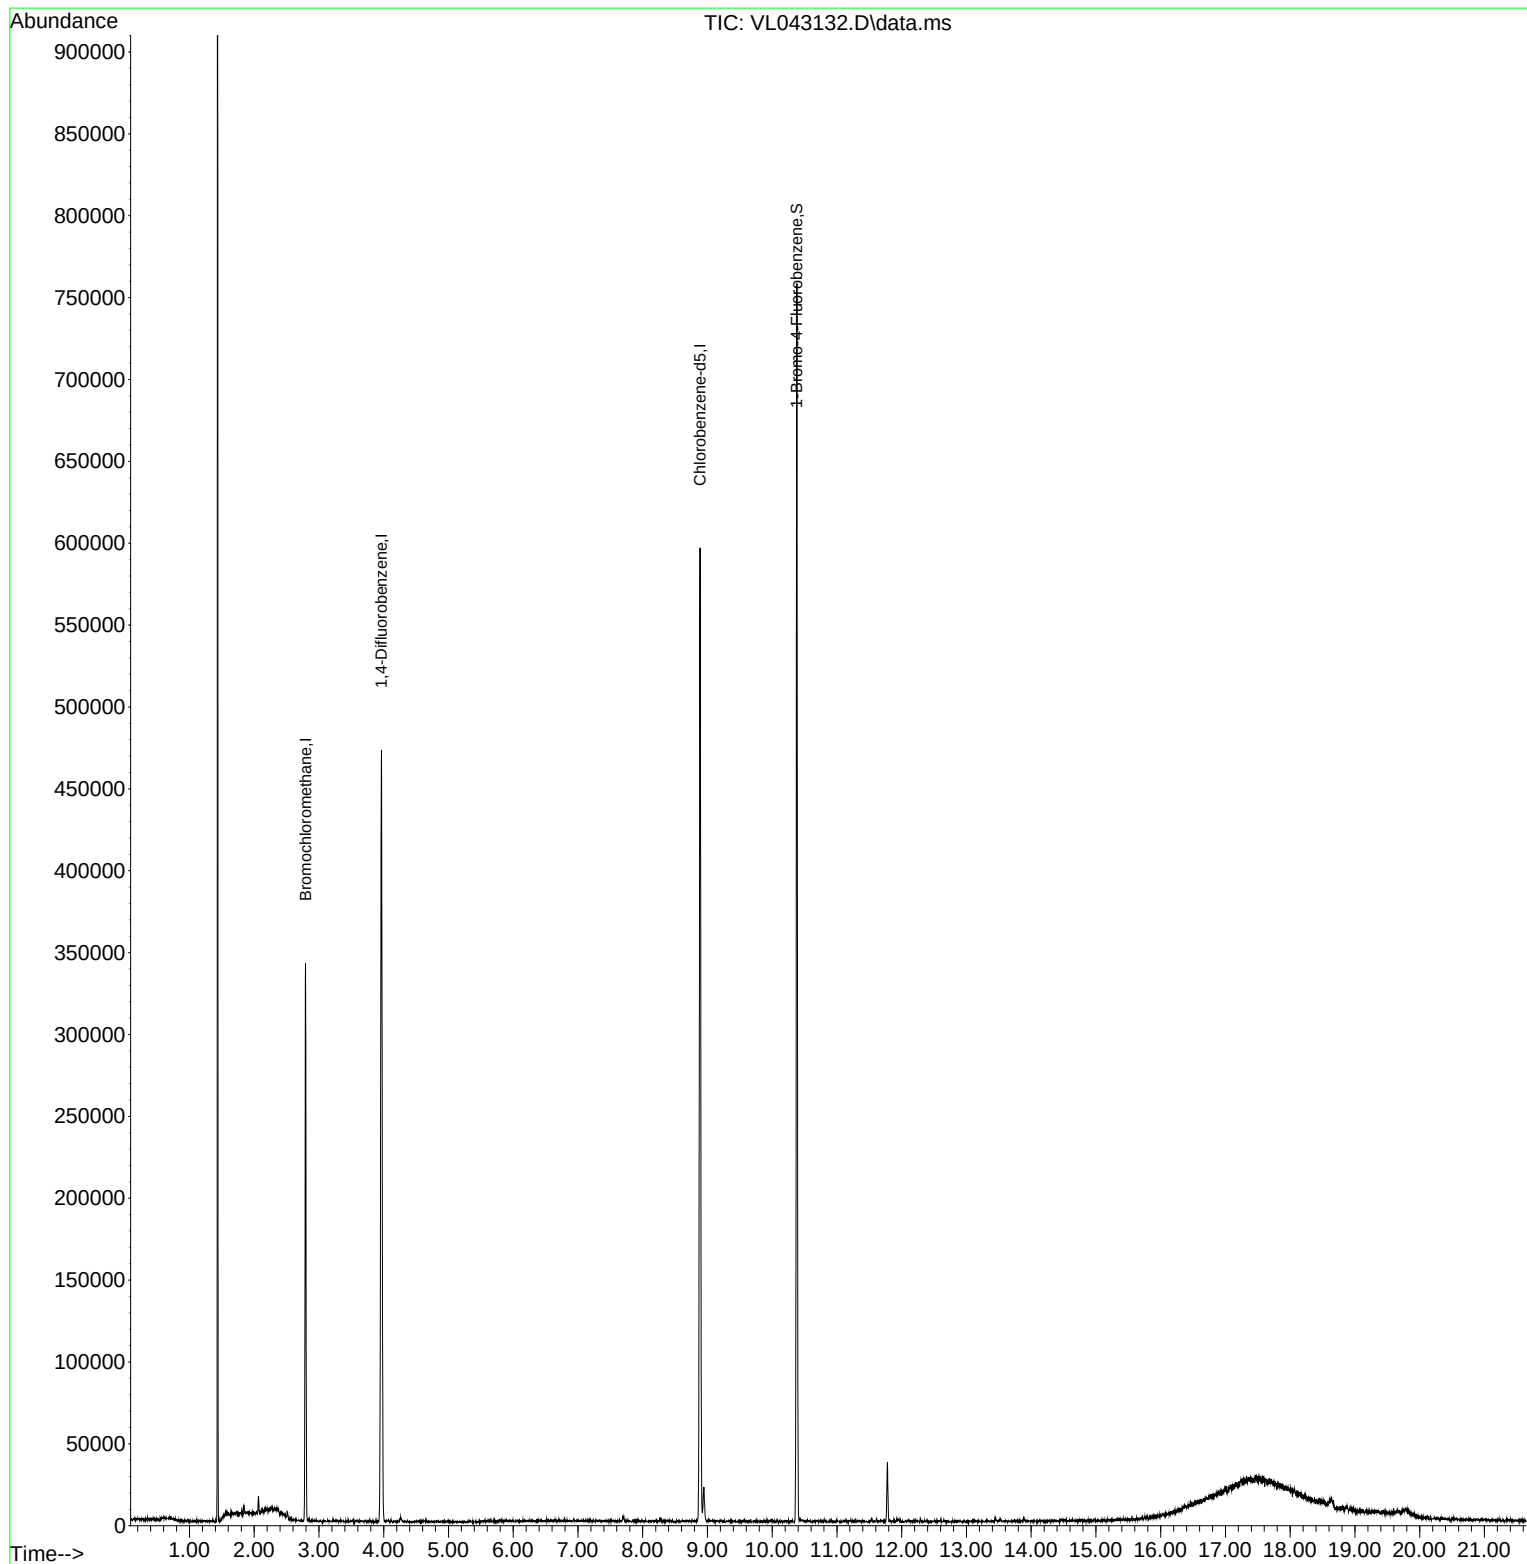


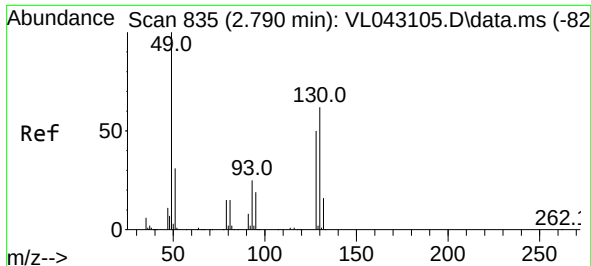

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.793 min Scan# 81
Delta R.T. 0.003 min
Lab File: VL043132.D
Acq: 17 Oct 2025 09:05




Instrument :
MSVOA_L
ClientSampleId :
VL1017ABL01


Tgt Ion: 49 Resp: 88811
Ion Ratio Lower Upper
49 100
128 48.5 24.4 73.4
130 63.5 31.0 93.0

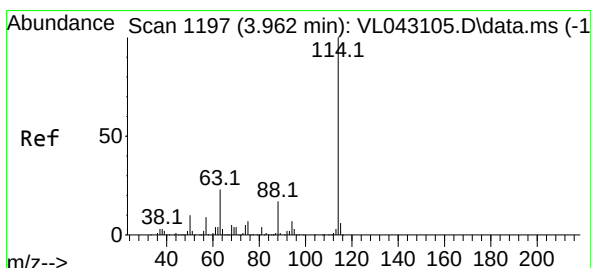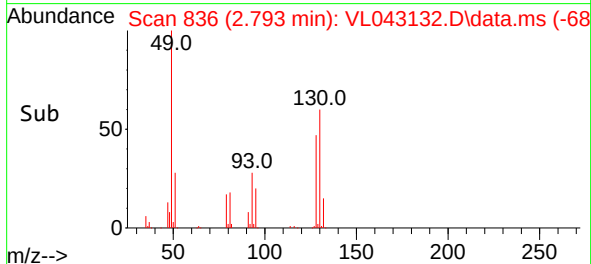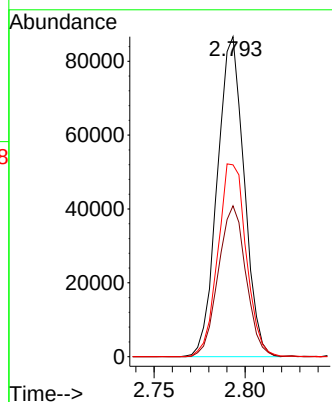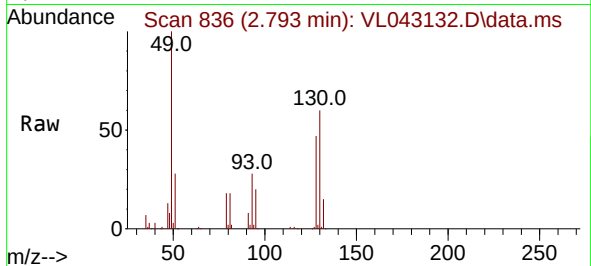

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.965 min Scan# 1198
Delta R.T. 0.003 min
Lab File: VL043132.D
Acq: 17 Oct 2025 09:05

Tgt Ion: 114 Resp: 284361
Ion Ratio Lower Upper
114 100
63 25.8 19.3 28.9
88 17.9 13.9 20.9


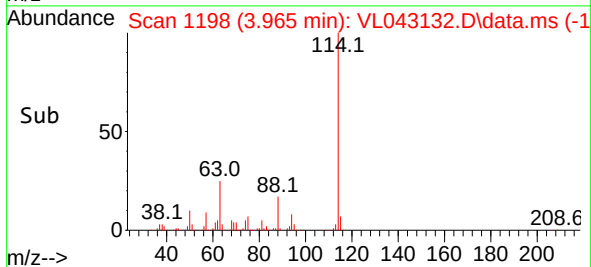
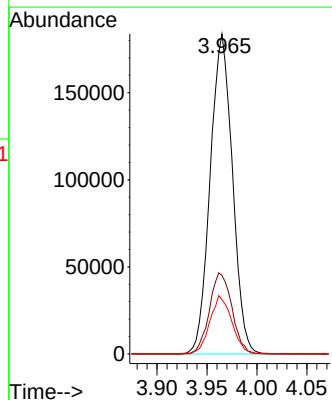
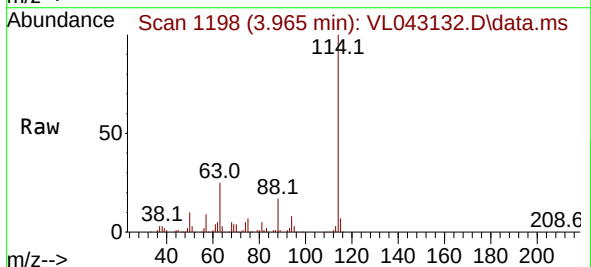


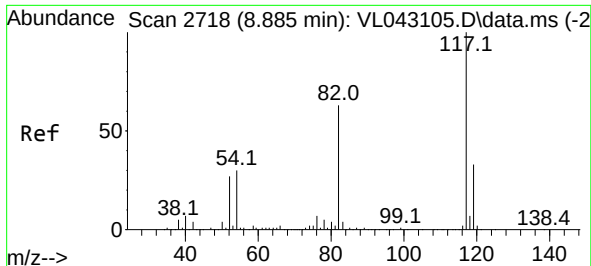

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.885 min Scan# 21
Delta R.T. -0.000 min
Lab File: VL043132.D
Acq: 17 Oct 2025 09:05

Instrument :
MSVOA_L
ClientSampleId :
VL1017ABL01

Tgt Ion:117 Resp: 240318
Ion Ratio Lower Upper
117 100
82 66.7 53.8 80.8
119 32.0 25.4 38.0

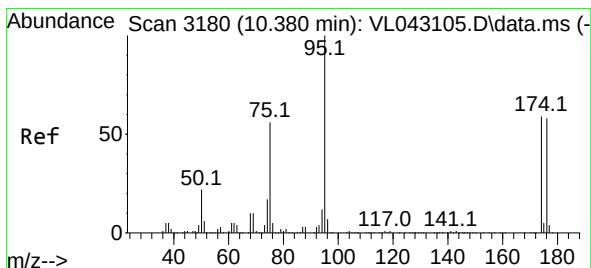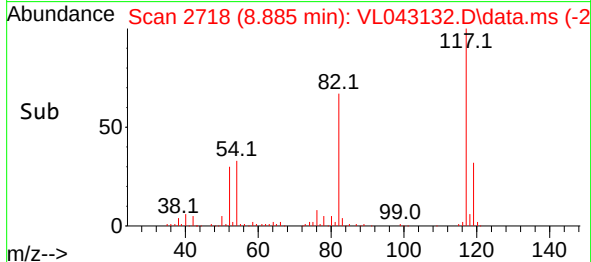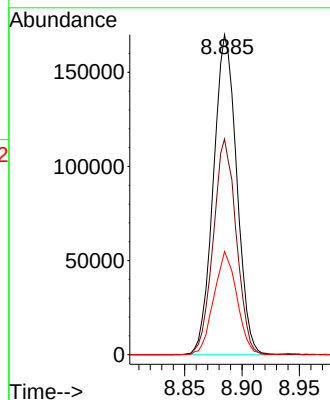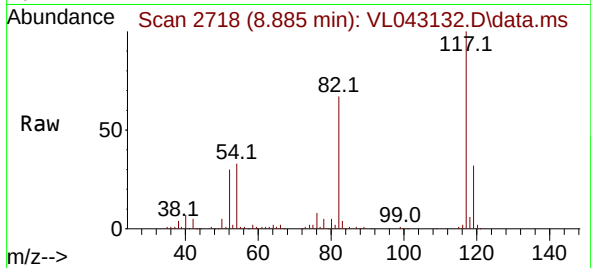

#68
1-Bromo-4-Fluorobenzene
Concen: 10.162 ppbv
RT: 10.380 min Scan# 3180
Delta R.T. -0.000 min
Lab File: VL043132.D
Acq: 17 Oct 2025 09:05

Tgt Ion: 95 Resp: 189815
Ion Ratio Lower Upper
95 100
174 58.8 48.3 72.5
175 4.2 3.8 5.8

