


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101821\
 Data File : VL037852.D
 Acq On : 18 Oct 2021 14:08
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

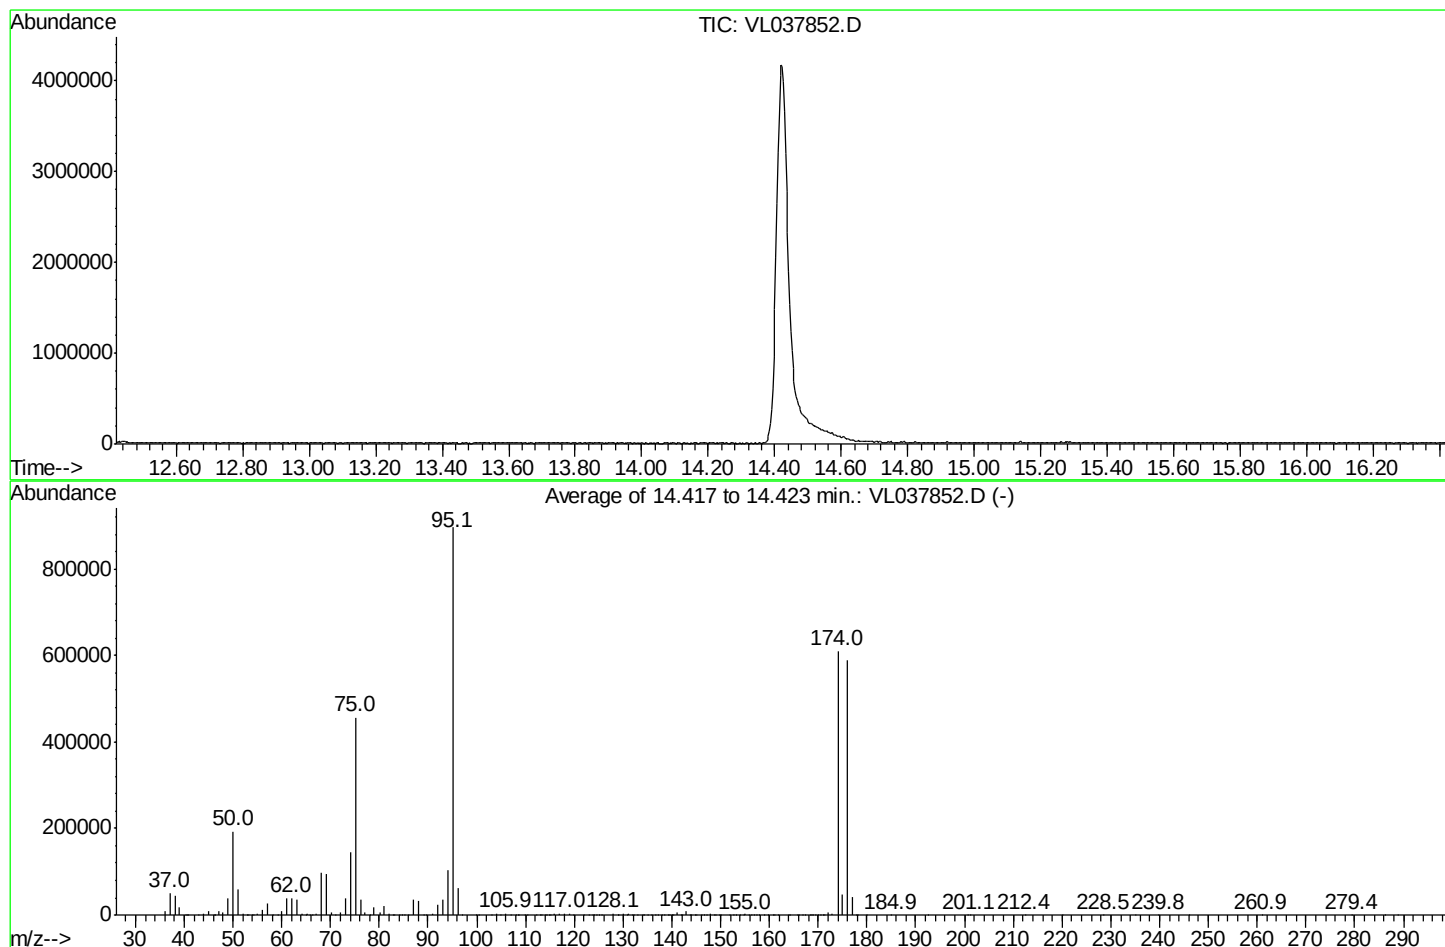

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.5	192469	PASS
75	95	30	66	50.8	455553	PASS
95	95	100	100	100.0	895893	PASS
96	95	5	9	6.9	61778	PASS
173	174	0.00	2	0.3	2100	PASS
174	95	50	120	68.0	609536	PASS
175	174	4	9	7.8	47360	PASS
176	174	93	101	96.5	588330	PASS
177	176	5	9	7.1	41645	PASS