


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL101920\  
 Data File : VL035789.D  
 Acq On : 19 Oct 2020 9:46  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400ml/MSVOA L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL092320AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Wed Sep 23 07:38:05 2020  
 Last Update : Wed Sep 23 07:38:05 2020

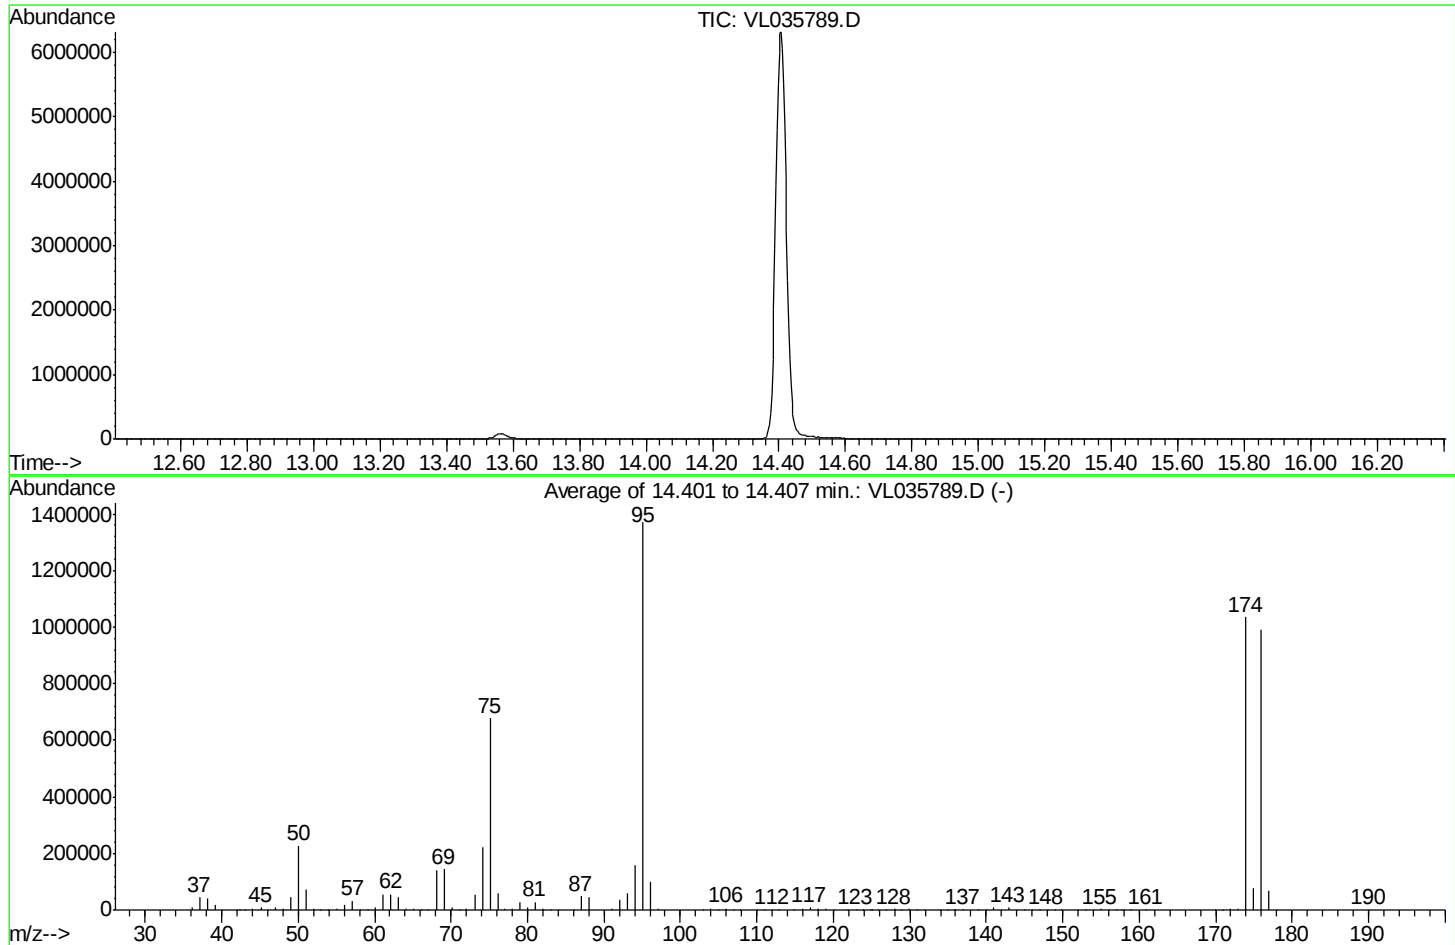

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3591

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 16.6      | 228074  | PASS             |
| 75          | 95           | 30           | 66           | 49.4      | 677226  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 1370282 | PASS             |
| 96          | 95           | 5            | 9            | 7.3       | 99568   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.6       | 5731    | PASS             |
| 174         | 95           | 50           | 120          | 75.5      | 1034410 | PASS             |
| 175         | 174          | 4            | 9            | 7.4       | 76298   | PASS             |
| 176         | 174          | 93           | 101          | 95.7      | 989440  | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 69133   | PASS             |