
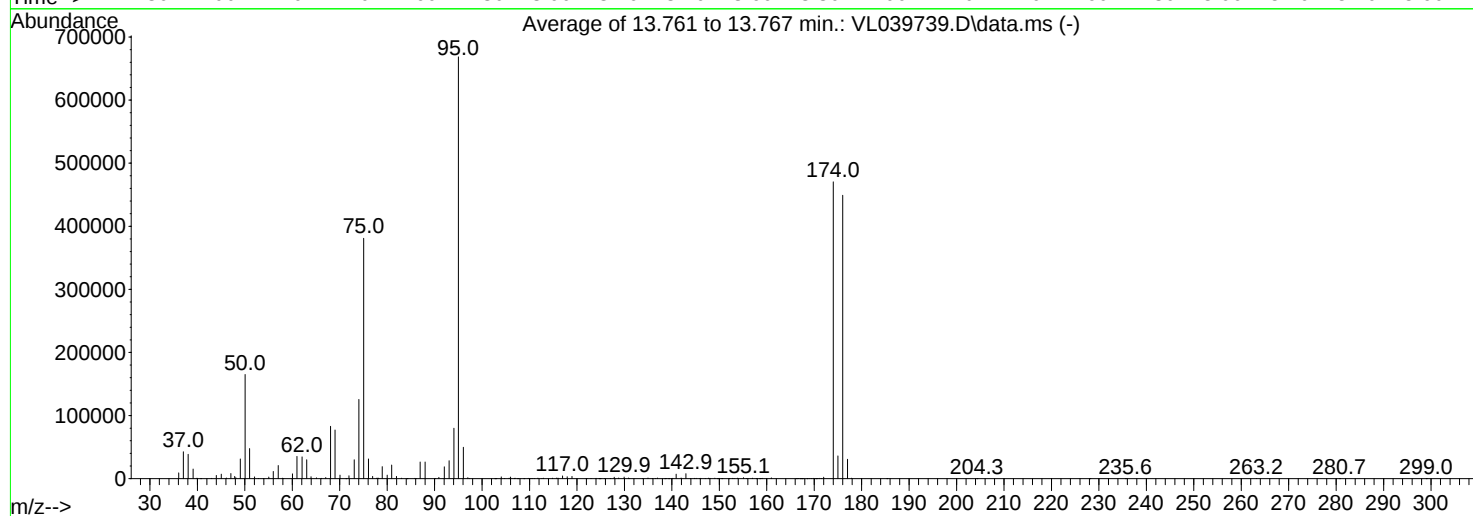


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102122\
 Data File : VL039739.D
 Acq On : 21 Oct 2022 9:16
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL102122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Sat Oct 22 02:12:34 2022

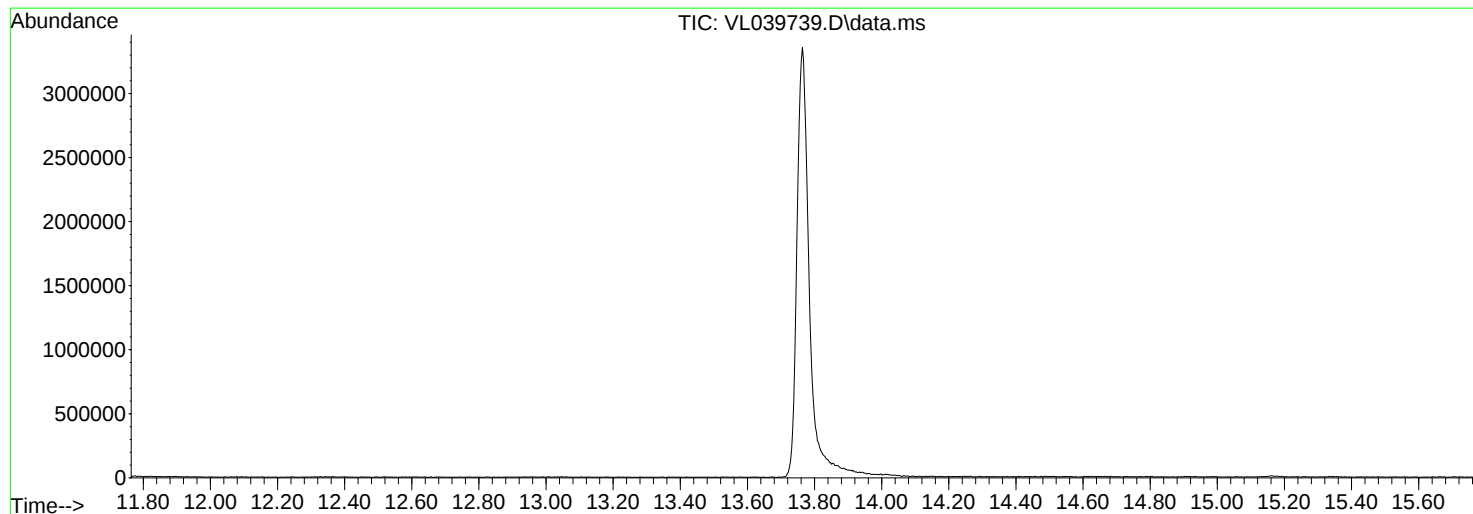

AutoFind: Scans 3470, 3471, 3472; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	165205	PASS
75	95	30	66	57.0	381035	PASS
95	95	100	100	100.0	668560	PASS
96	95	5	9	7.4	49627	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.4	470464	PASS
175	174	4	9	7.7	36157	PASS
176	174	93	101	95.5	449152	PASS
177	176	5	9	6.9	30811	PASS

Average of 13.761 to 13.767 min.: VL039739.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9117	47.85	3693	57.90	694	69.00	7715
37.05	42528	48.10	1526	58.20	284	70.05	548
38.05	38459	49.05	31333	60.05	7660	71.30	14
39.10	15159	50.05	165205	61.00	35240	71.95	458
39.90	858	51.00	47792	62.05	34555	73.05	30003
40.70	96	52.05	2711	63.05	29899	74.05	125523
43.00	555	52.90	238	63.95	3034	75.05	381035
44.00	5203	53.95	202	65.10	1330	76.05	31163
45.05	7116	55.05	2580	66.15	464	76.95	3488
46.10	939	56.00	11454	67.05	1912	77.80	697
47.05	8239	57.05	20715	68.05	83032	78.00	890

Average of 13.761 to 13.767 min.: VL039739.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.20	887	90.15	299	104.05	2841	110.70	328
78.95	18973	90.90	2029	104.75	293	111.10	316
80.00	5568	92.05	18797	105.70	713	111.75	756
80.95	21520	93.05	28499	106.00	2467	112.60	197
81.95	3678	94.05	79928	106.80	332	112.90	680
83.05	696	95.00	668560	106.95	686	114.85	844
84.20	65	96.05	49627	107.50	71	115.75	957
85.85	555	97.00	1481	108.80	70	116.00	691
86.10	174	97.30	408	109.70	570	116.95	4268
86.95	26344	102.70	116	110.00	209	117.95	3110
88.00	26381	102.90	91	110.30	160	118.95	3460

Average of 13.761 to 13.767 min.: VL039739.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.90	57	131.10	259	140.90	7091	149.05	760
122.95	389	133.85	179	141.95	911	149.60	137
124.00	549	134.95	905	142.95	7840	149.95	581
124.65	142	135.90	371	143.95	291	150.50	78
124.90	77	136.60	189	144.75	487	152.00	124
125.80	327	136.95	1126	145.10	615	152.80	574
127.05	277	138.50	127	145.90	231	153.10	219
127.85	2375	138.90	219	146.10	618	153.90	731
128.80	1126	139.30	61	147.05	329	155.10	1414
129.95	2624	140.00	415	147.75	779	155.75	220
130.85	1091	140.20	443	148.00	529	156.00	176

Average of 13.761 to 13.767 min.: VL039739.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.00	830	168.50	157	175.00	36157		
157.80	156	169.05	296	176.00	449152		
158.50	156	169.40	292	177.00	30811		
158.80	402	169.80	462	177.90	777		
159.05	485	170.20	183	185.30	126		
160.95	1221	170.40	90	204.30	72		
166.25	154	170.75	371	228.10	52		
166.70	215	171.05	530	235.60	96		
167.00	62	171.50	280	263.20	162		
167.30	92	172.00	2426	280.70	142		
167.50	58	174.00	470464	299.00	87		