


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL102418\
Data File : VL032685.D
Acq On : 24 Oct 2018 13:23
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL101818AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 25 05:15:43 2018
Last Update : Thu Oct 25 05:15:43 2018

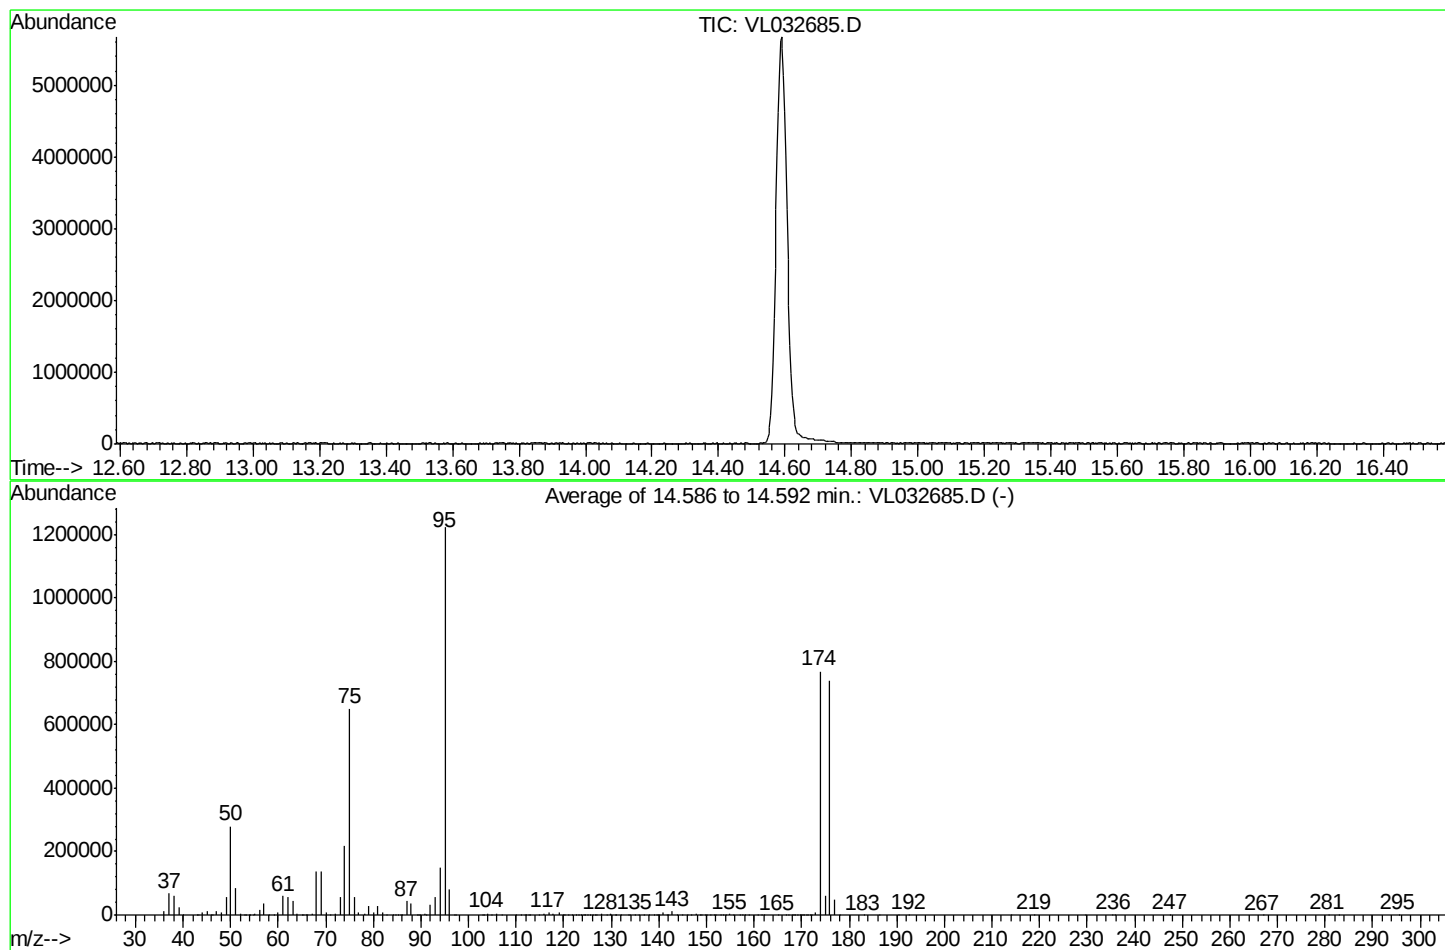

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	279445	PASS
75	95	30	66	53.3	651861	PASS
95	95	100	100	100.0	1222826	PASS
96	95	5	9	6.7	81850	PASS
173	174	0.00	2	1.1	8818	PASS
174	95	50	120	62.8	767530	PASS
175	174	4	9	7.9	60344	PASS
176	174	93	101	96.3	739413	PASS
177	176	5	9	6.6	48898	PASS