

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL102521\
Data File : VL037892.D
Acq On : 25 Oct 2021 13:31
Operator : SY/AP
Sample : OC102221 CAN 10297
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC102221 CAN 10297

Quant Time: Oct 27 12:03:48 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
QLast Update : Mon Oct 04 17:43:54 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1424328	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.19	114	4209307	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.10	117	3537598	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	2515283	10.17	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.70%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL102521\
Data File : VL037892.D
Acq On : 25 Oct 2021 13:31
Operator : SY/AP
Sample : OC102221 CAN 10297
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC102221 CAN 10297

Quant Time: Oct 27 12:03:48 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL100421AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
QLast Update : Mon Oct 04 17:43:54 2021
Response via : Initial Calibration

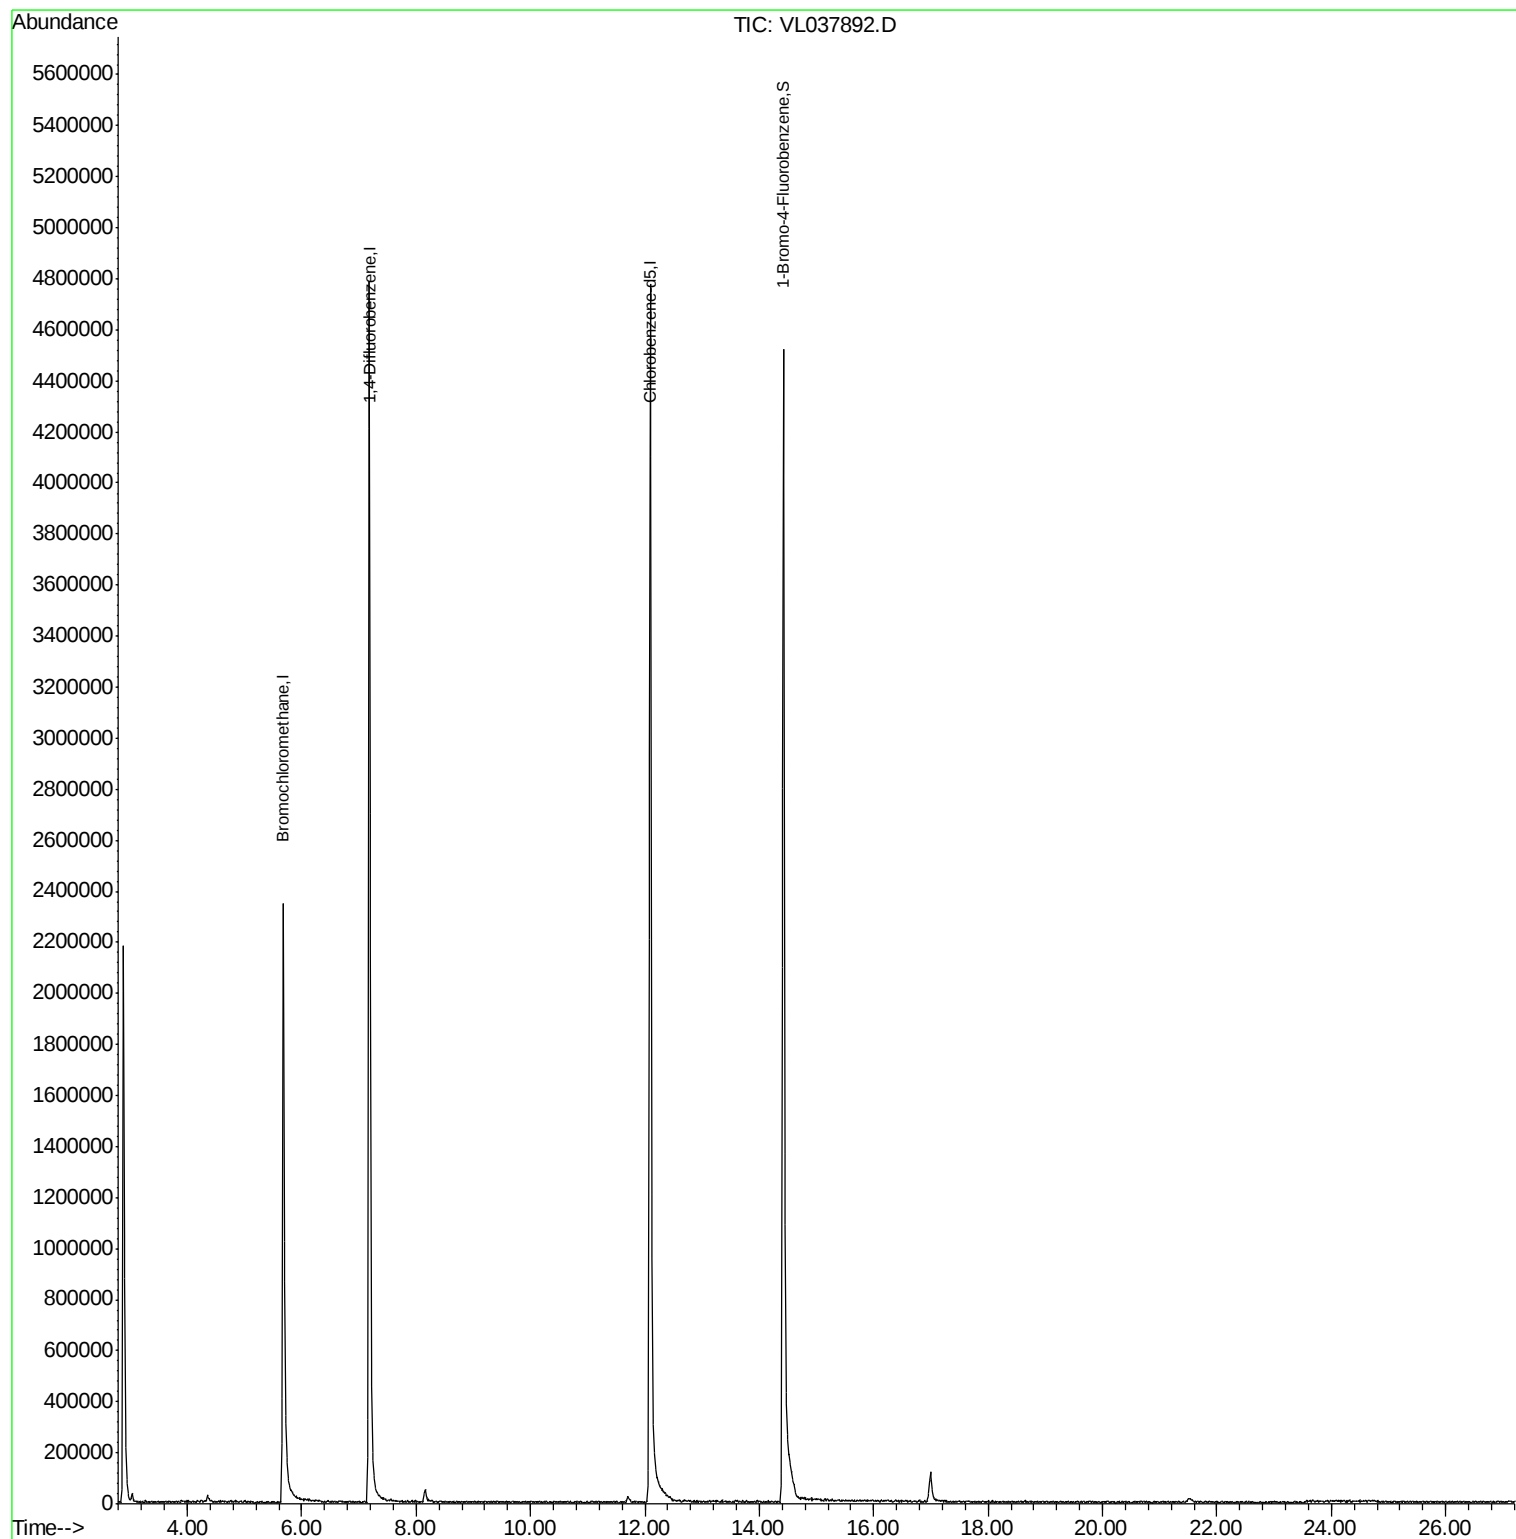

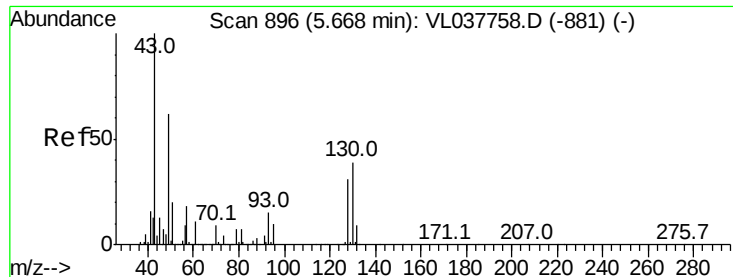

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.67

Delta R.T. MSVOA_1

Lab File: ClientSampleId:

QC102221 CAN 10297

Acq: 25 Oct 2021 13:31


Tot Ion: 49 Resp: 1424328

Ion Ratio Lower Upper

49 100

128 53.9 27.1 81.3




130 70.2 33.2 99.6

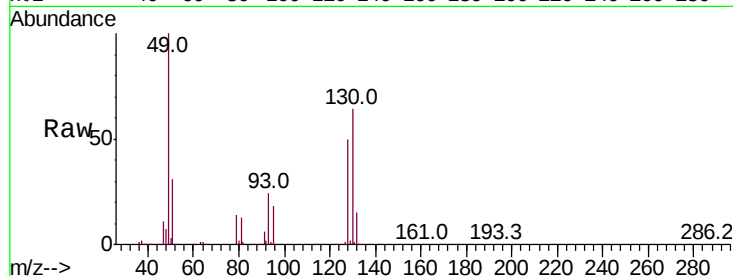

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

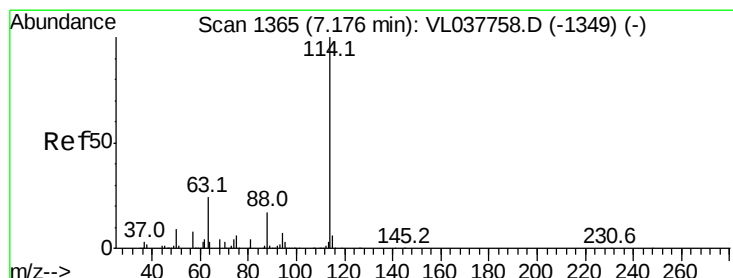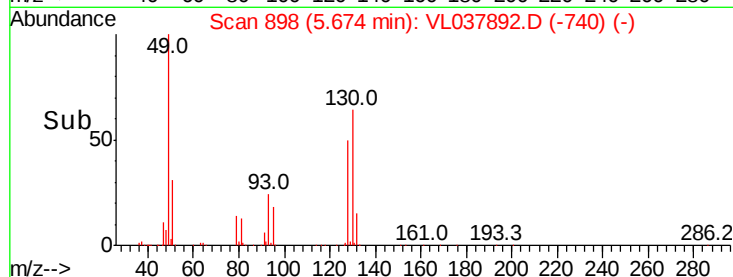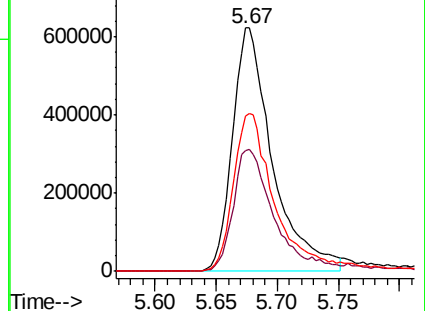

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.19 min Scan# 1368

Delta R.T. 0.01 min

Lab File: VL037892.D

Acq: 25 Oct 2021 13:31


Tgt Ion: 114 Resp: 4209307

Ion Ratio Lower Upper

114 100

63 23.9 19.4 29.2



88 18.0 14.4 21.6

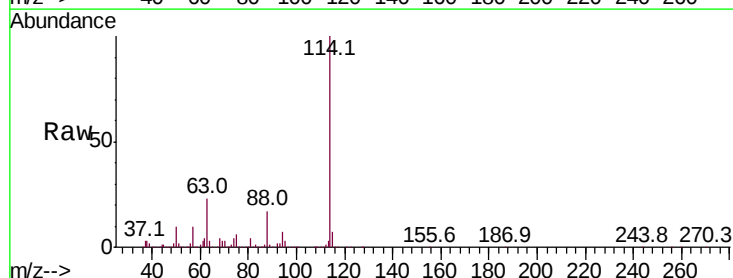


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



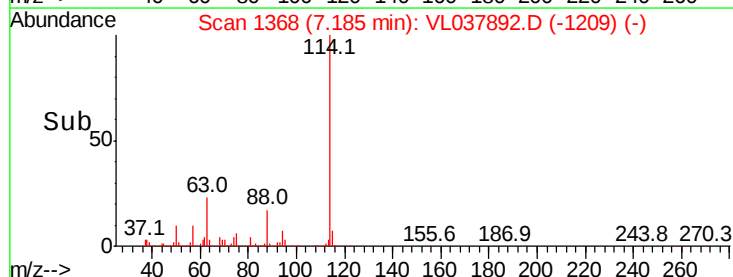
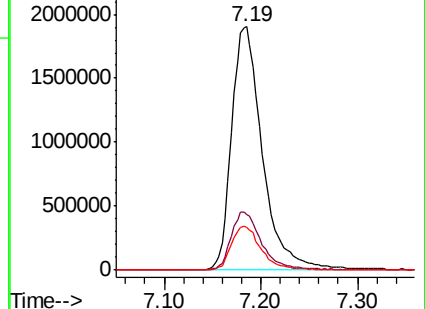


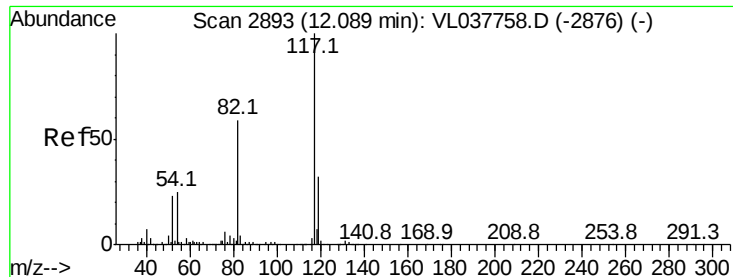

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.10 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
QC102221 CAN 10297
Acq: 25 Oct 2021 13:31

Tot Ion: 117 Resp: 3537598

Ion	Ratio	Lower	Upper
117	100		
82	64.0	52.2	78.2
119	33.9	26.0	39.0

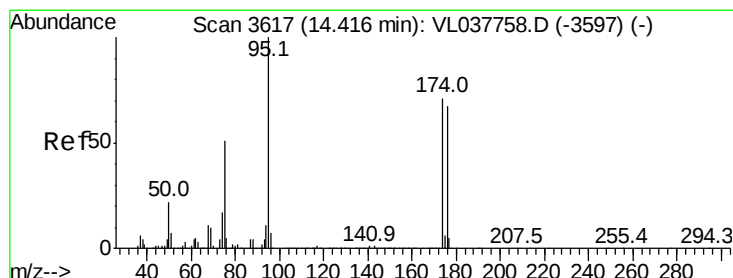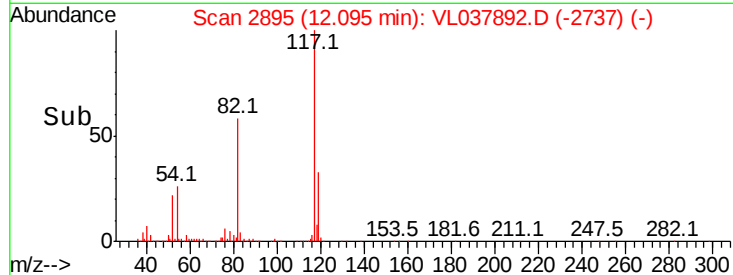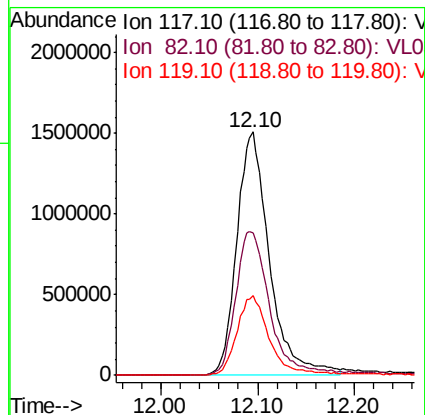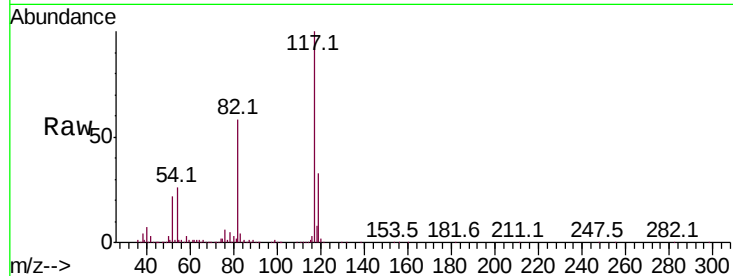

#68
1-Bromo-4-Fluorobenzene
Concen: 10.167 ppbv
RT: 14.42 min Scan# 3619
Delta R.T.: 0.01 min
Lab File: VL037892.D
Acq: 25 Oct 2021 13:31

Tgt Ion: 95 Resp: 2515283

Ion	Ratio	Lower	Upper
95	100		
174	72.9	57.8	86.6
175	5.5	4.7	7.1

