


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL102521\
 Data File : VL037888.D
 Acq On : 25 Oct 2021 9:58
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL100421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Oct 04 17:43:54 2021
 Last Update : Mon Oct 04 17:43:54 2021

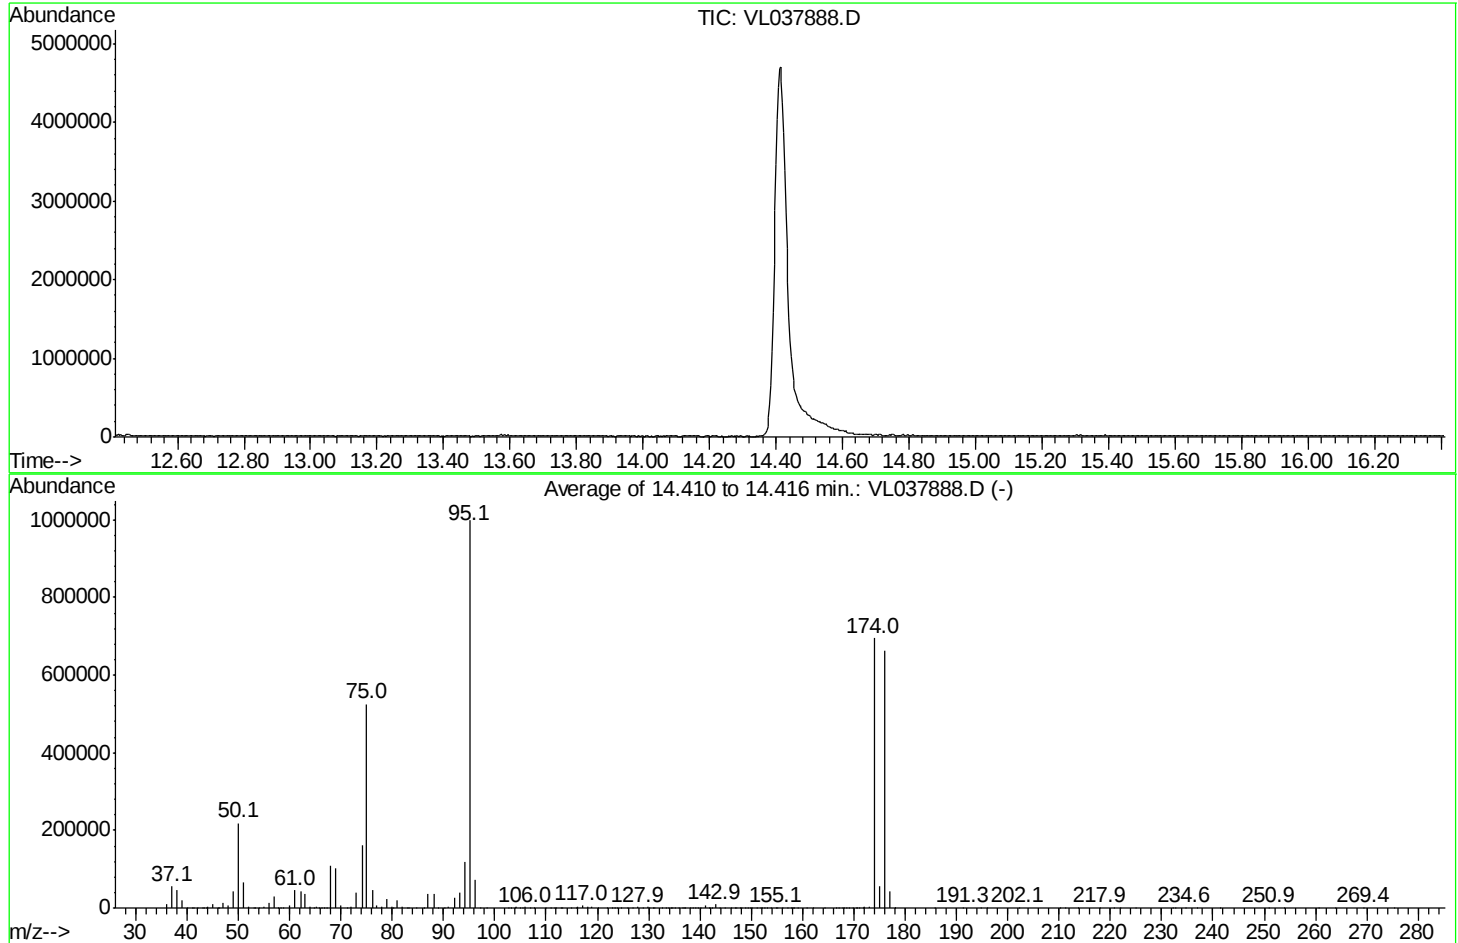

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.9	218261	PASS
75	95	30	66	52.6	525443	PASS
95	95	100	100	100.0	998570	PASS
96	95	5	9	7.2	71901	PASS
173	174	0.00	2	0.5	3561	PASS
174	95	50	120	69.7	695573	PASS
175	174	4	9	7.9	55069	PASS
176	174	93	101	95.1	661248	PASS
177	176	5	9	6.6	43813	PASS