
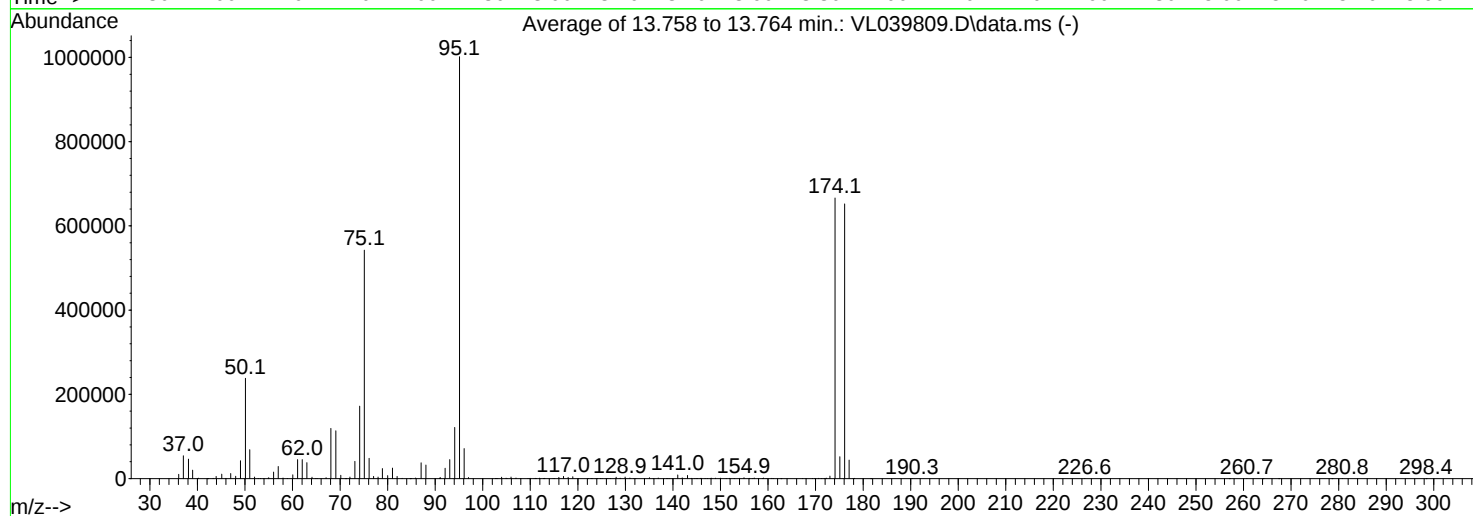


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110222\
 Data File : VL039809.D
 Acq On : 2 Nov 2022 10:05
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Nov 03 09:27:12 2022

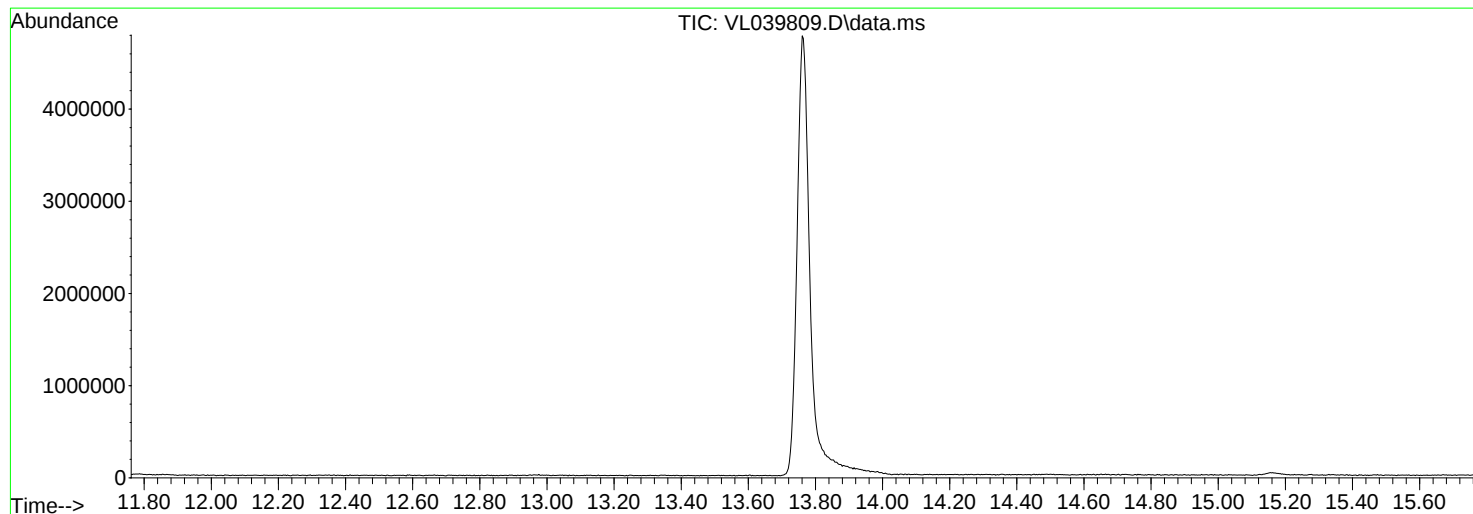

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	237973	PASS
75	95	30	66	54.1	542357	PASS
95	95	100	100	100.0	1001600	PASS
96	95	5	9	7.1	71189	PASS
173	174	0.00	2	0.9	5767	PASS
174	95	50	120	66.5	666240	PASS
175	174	4	9	7.8	51859	PASS
176	174	93	101	97.9	652288	PASS
177	176	5	9	6.7	43795	PASS

Average of 13.758 to 13.764 min.: VL039809.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	10081	48.05	5452	57.00	28622	68.05	11932
37.05	54098	49.05	42277	58.00	1384	69.10	11353
38.10	46229	50.10	237973	58.90	91	70.15	7805
39.00	19922	51.00	68718	60.05	8802	71.15	3603
40.20	1075	52.00	3467	61.05	44891	72.05	40757
42.10	51	52.80	254	62.05	44901	73.10	171782
43.30	497	53.30	237	63.00	37783	74.10	542357
43.95	5200	53.95	370	64.10	3149	75.10	47952
45.10	10549	54.90	1227	64.90	253	76.10	5130
46.00	516	55.00	1883	65.15	216	77.05	3560
47.00	12131	56.00	15267	67.05	2170	78.00	

Average of 13.758 to 13.764 min.: VL039809.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	23974	91.10	2139	104.90	1087	112.80	140
80.00	7129	92.10	24507	105.10	302	112.90	302
81.00	24852	93.05	45083	105.95	3651	113.05	531
82.00	5173	94.10	121507	107.00	1229	114.80	256
83.05	776	95.10	1.0016e+006	108.00	77	115.15	204
84.70	54	96.10	71189	109.50	86	116.00	2870
84.95	132	97.00	2499	109.95	662	117.00	5089
85.90	1159	102.70	154	110.80	242	117.95	2937
87.05	37448	102.90	186	111.10	830	118.95	4258
88.05	31992	103.15	255	111.30	171	120.10	271
90.90	1380	103.95	3096	111.95	834	122.20	105

Average of 13.758 to 13.764 min.: VL039809.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.80	101	129.95	3509	139.20	156	146.75	307
123.00	90	130.95	1467	139.95	381	147.25	342
123.80	137	131.80	82	141.00	8472	147.90	507
124.15	426	132.20	122	141.95	1638	148.15	1017
124.75	293	134.00	161	143.05	7544	148.95	893
125.10	413	135.05	2066	143.90	677	150.00	906
125.95	423	135.85	201	144.60	74	151.20	146
126.30	81	136.90	1495	144.90	368	151.90	523
126.80	79	138.10	77	145.20	210	152.90	396
128.05	3241	138.70	72	145.75	628	153.95	783
128.90	987	138.90	110	146.00	464	154.95	1929

Average of 13.758 to 13.764 min.: VL039809.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.10	518	168.00	158	175.10	51859	267.40	56
156.80	367	169.35	200	176.10	652288	278.60	57
157.10	1299	169.80	203	177.05	43795	280.80	71
158.00	261	170.00	370	177.90	262	298.40	54
158.80	235	170.65	743	178.20	635		
159.05	1238	171.30	294	181.60	54		
159.60	104	171.80	248	190.30	101		
160.80	508	172.00	490	226.60	74		
161.10	372	172.30	895	257.00	63		
162.70	55	173.00	5767	260.70	186		
167.30	103	174.10	666240	264.10	55		