
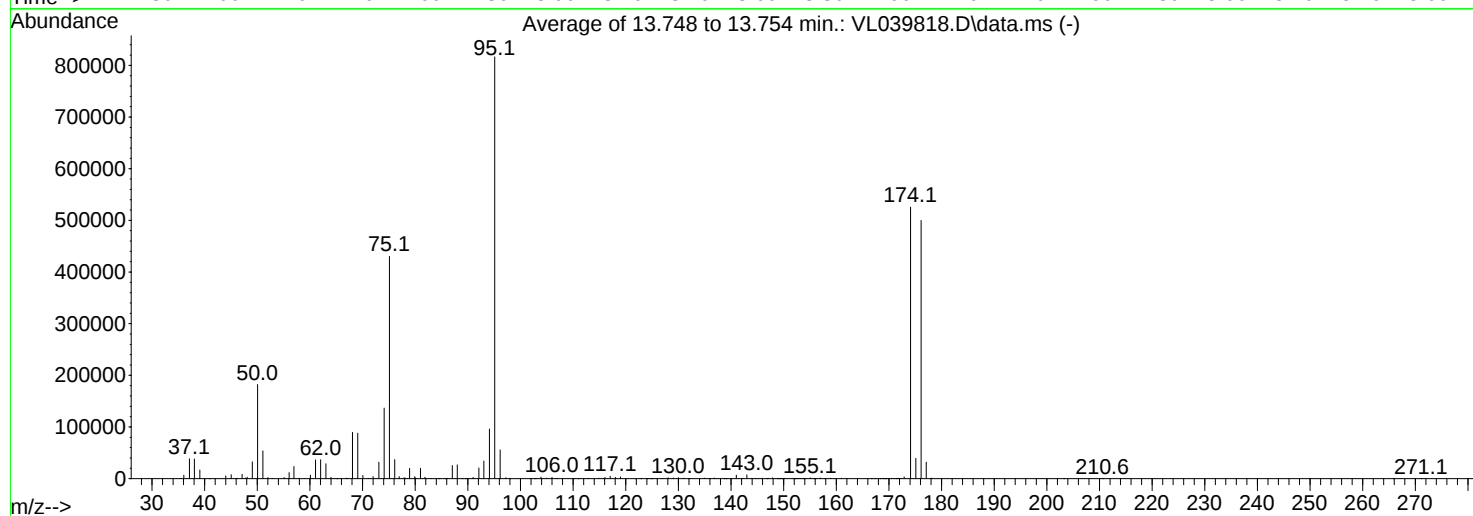


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110322\
 Data File : VL039818.D
 Acq On : 3 Nov 2022 8:26
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Nov 03 09:27:12 2022

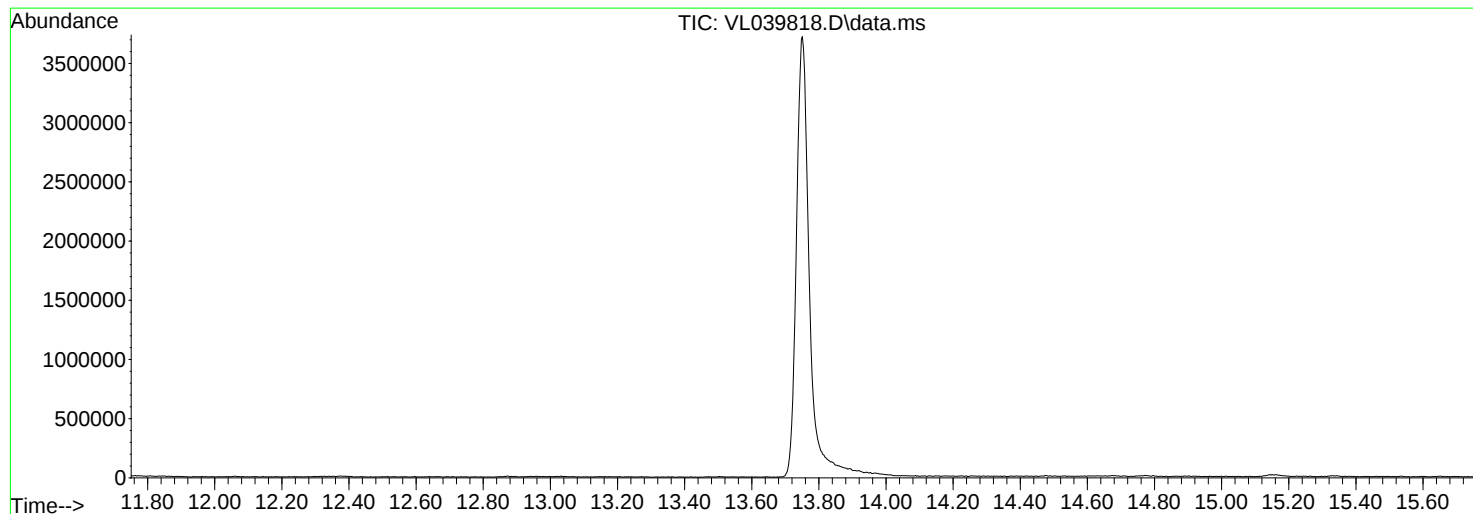

AutoFind: Scans 3466, 3467, 3468; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.3	182187	PASS
75	95	30	66	52.7	430251	PASS
95	95	100	100	100.0	816512	PASS
96	95	5	9	6.8	55731	PASS
173	174	0.00	2	0.7	3528	PASS
174	95	50	120	64.4	525760	PASS
175	174	4	9	7.5	39224	PASS
176	174	93	101	95.1	500053	PASS
177	176	5	9	6.4	31947	PASS

Average of 13.748 to 13.754 min.: VL039818.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6912	47.80	1345	60.10	6919	71.10	231
37.10	38373	48.10	2738	61.05	36219	72.00	414
38.05	38029	49.05	32448	62.05	36448	73.10	3188
39.10	16829	50.05	182187	63.05	28776	74.10	13674
40.00	690	51.05	53947	64.00	2653	75.10	430251
40.90	42	52.05	2167	65.10	52	76.10	37003
44.00	5191	52.90	225	66.90	854	76.95	4002
45.05	7809	55.10	2069	67.20	670	77.70	416
45.90	181	56.05	11661	68.10	89672	77.90	1744
46.25	598	56.95	23531	69.10	88093	78.20	804
47.10	8517	57.95	926	70.05	6239	78.95	19821

Average of 13.748 to 13.754 min.: VL039818.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	3770	88.90	171	102.70	61	111.15	325
80.10	1702	89.55	154	103.10	284	111.95	543
81.00	20213	91.00	2346	103.90	3245	112.80	243
81.85	2825	92.10	20627	104.10	669	112.95	411
82.10	234	93.05	34091	105.00	836	114.90	982
83.05	432	94.10	96077	106.00	2496	115.75	474
84.50	125	95.10	816512	106.85	387	116.05	2063
85.70	143	96.15	55731	107.10	342	117.05	4522
86.15	746	97.25	1819	109.90	366	118.05	2541
87.05	25565	98.00	129	110.10	93	119.00	3547
88.00	26637	101.90	57	110.90	133	121.80	105

Average of 13.748 to 13.754 min.: VL039818.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.85	141	131.05	868	141.95	670	148.80	174
124.10	173	132.00	99	142.20	333	149.10	179
124.70	80	135.05	1315	143.00	7515	149.40	63
125.00	76	135.85	195	143.95	727	149.70	132
125.80	208	136.10	199	144.70	592	150.15	513
126.00	294	136.80	1358	145.15	388	151.75	246
126.90	299	137.20	238	145.80	278	152.20	55
127.80	779	138.70	100	146.00	885	152.70	210
128.10	1666	139.05	176	146.80	62	152.90	216
129.05	1367	140.00	269	147.05	577	153.15	399
130.00	2007	141.00	6733	147.90	1531	153.60	78

Average of 13.748 to 13.754 min.: VL039818.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.00	179	168.80	113	174.10	525760		
155.05	1660	169.20	62	175.10	39224		
155.75	184	169.40	87	176.10	500053		
156.00	140	170.00	505	177.10	31947		
156.95	1156	170.50	196	177.90	167		
157.80	76	170.80	282	178.15	1203		
158.95	897	171.15	457	203.20	58		
160.95	880	171.40	165	210.60	109		
166.65	156	171.80	549	265.80	90		
167.30	127	172.30	407	271.10	141		
168.30	147	172.90	3528				