


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL110420\
 Data File : VL035827.D
 Acq On : 4 Nov 2020 8:21
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020
 Last Update : Wed Nov 04 02:40:06 2020

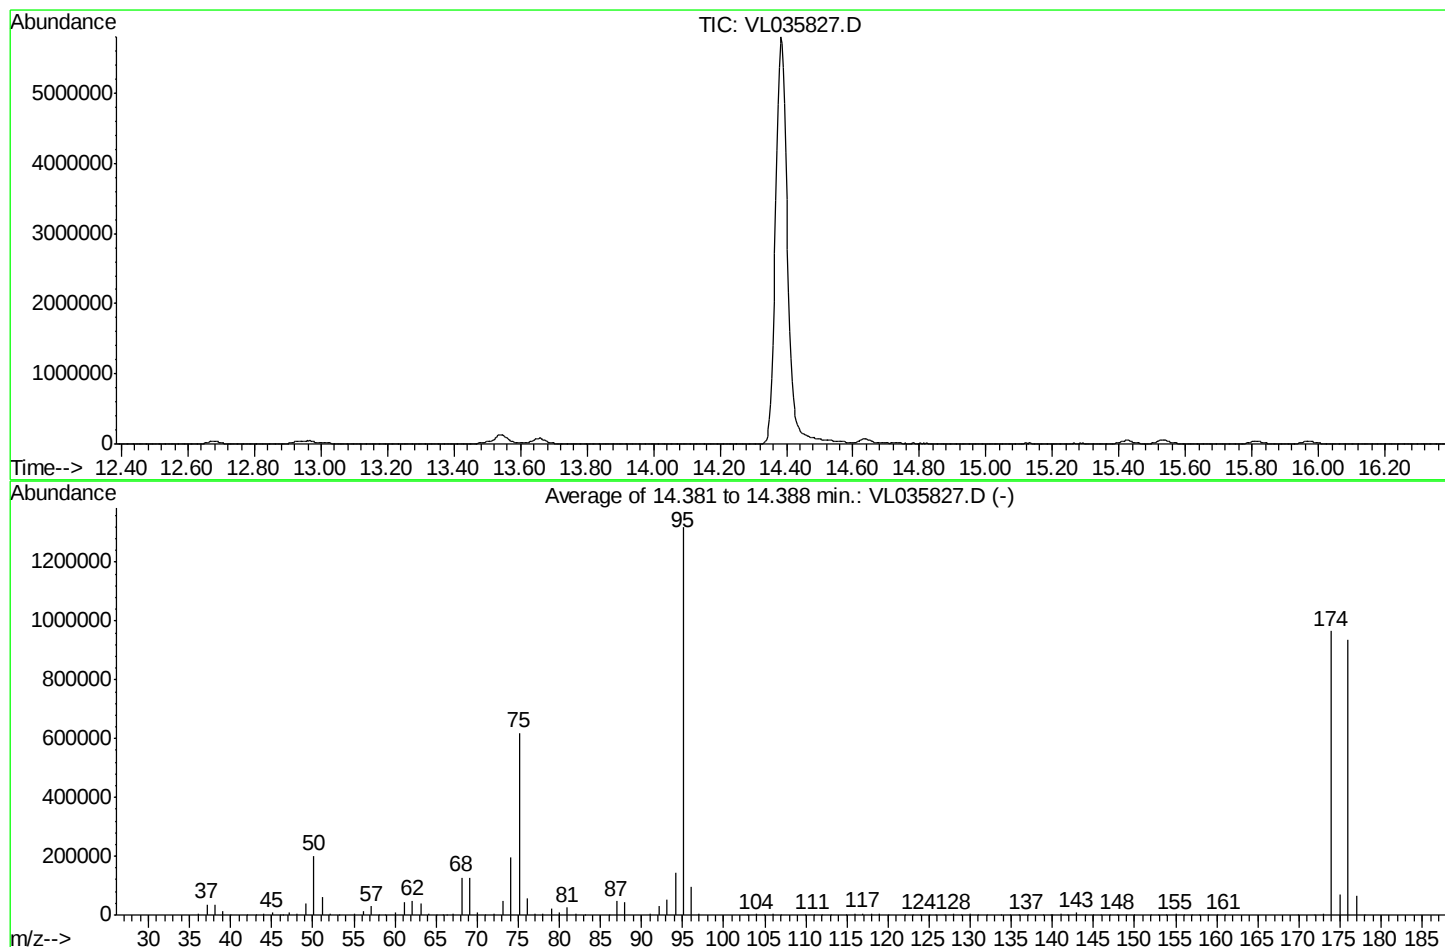

AutoFind: Scans 3606, 3607, 3608; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	15.3	201792	PASS
75	95	30	66	47.1	620693	PASS
95	95	100	100	100.0	1318912	PASS
96	95	5	9	7.4	97413	PASS
173	174	0.00	2	0.5	5294	PASS
174	95	50	120	73.2	965696	PASS
175	174	4	9	7.1	68938	PASS
176	174	93	101	96.8	934698	PASS
177	176	5	9	6.9	64840	PASS