
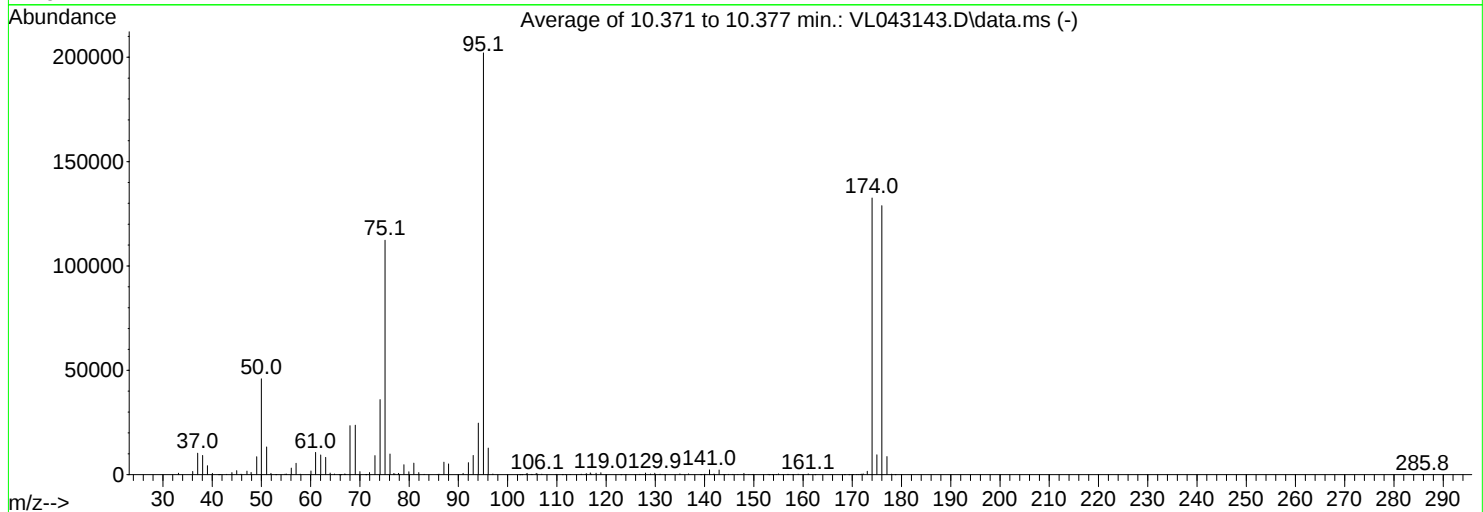


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110425\
Data File : VL043143.D
Acq On : 04 Nov 2025 07:41
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 15 02:12:58 2025

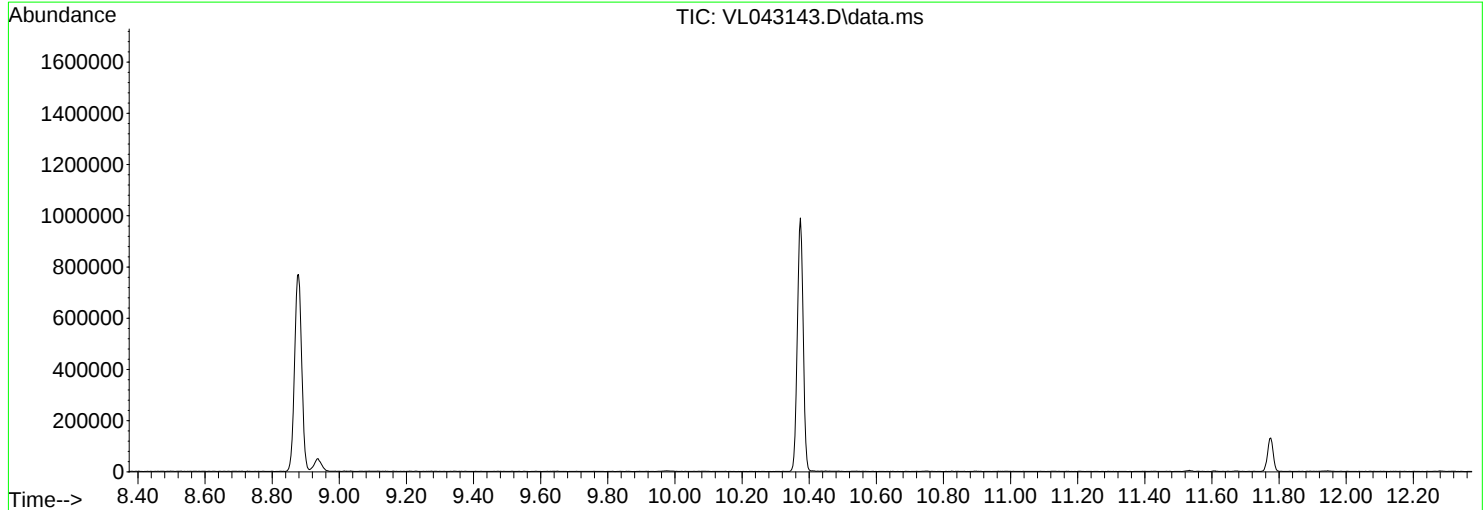

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3159

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.7	45960	PASS
75	95	30	66	55.6	112355	PASS
95	95	100	100	100.0	202112	PASS
96	95	5	9	6.3	12701	PASS
173	174	0.00	2	1.2	1639	PASS
174	95	50	120	65.6	132573	PASS
175	174	4	9	7.2	9530	PASS
176	174	93	101	97.2	128885	PASS
177	176	5	9	6.8	8708	PASS

Average of 10.371 to 10.377 min.: VL043143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	659	45.85	208	57.05	5432	67.10	231
36.05	1506	47.05	1659	57.90	255	68.00	2348
37.05	10299	47.90	1084	60.05	1734	69.05	2371
38.05	9177	49.05	8567	61.00	10656	70.00	150
39.05	4290	50.00	45960	62.05	9420	71.20	17
40.05	601	51.05	13302	63.05	8309	71.95	1001
41.30	19	51.95	589	63.95	754	73.05	9161
41.70	60	52.90	41	64.85	343	74.10	35933
42.95	164	54.80	271	65.80	21	75.10	112355
44.00	1026	55.05	313	66.10	19	76.10	9857
45.00	1952	56.05	3191	66.90	287	76.85	465

Average of 10.371 to 10.377 min.: VL043143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.10	388	88.00	5147	103.95	647	115.90	243
77.85	614	90.95	612	104.80	145	116.05	488
78.10	165	92.05	5788	105.00	79	116.80	815
78.95	4721	93.00	9198	105.80	597	117.00	253
79.95	1405	94.05	24725	106.10	332	117.95	675
80.95	5553	95.10	202112	106.95	208	118.95	944
81.95	1038	96.05	12701	109.85	173	120.05	48
83.05	143	97.00	272	111.10	21	123.00	26
85.70	64	102.50	36	111.80	116	123.85	77
86.05	257	102.90	17	112.70	70	124.10	59
87.05	5959	103.80	322	114.95	229	125.90	71

Average of 10.371 to 10.377 min.: VL043143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.85	134	141.90	311	151.95	83	161.05	383
128.00	763	142.95	2210	152.90	175	162.40	20
129.00	303	143.80	103	153.10	27	165.65	84
129.90	694	144.00	46	153.80	37	168.40	21
130.95	215	144.85	174	154.60	51	169.30	19
131.90	19	145.75	181	155.00	376	170.20	79
135.00	408	146.75	94	155.90	52	170.85	63
136.75	364	148.00	603	156.85	127	171.20	79
139.20	23	149.00	106	157.10	142	171.60	166
140.05	223	149.80	96	157.90	25	171.90	270
141.00	2334	149.95	171	159.00	218	172.20	400

Average of 10.371 to 10.377 min.: VL043143.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.05	1639						
174.00	132573						
175.00	9530						
176.00	128885						
177.05	8708						
178.00	222						
178.70	21						
285.80	18						

Instrument :

MSVOA_L

ClientSampleId :

BFB