
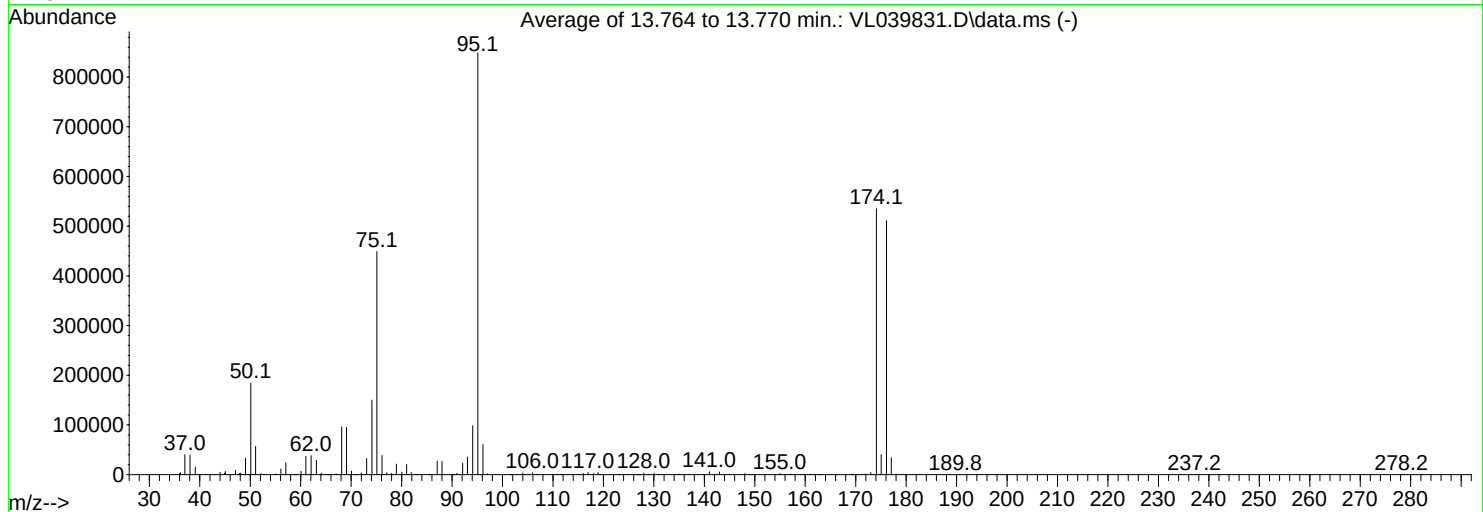


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110722\
 Data File : VL039831.D
 Acq On : 7 Nov 2022 8:27
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Nov 03 09:27:12 2022

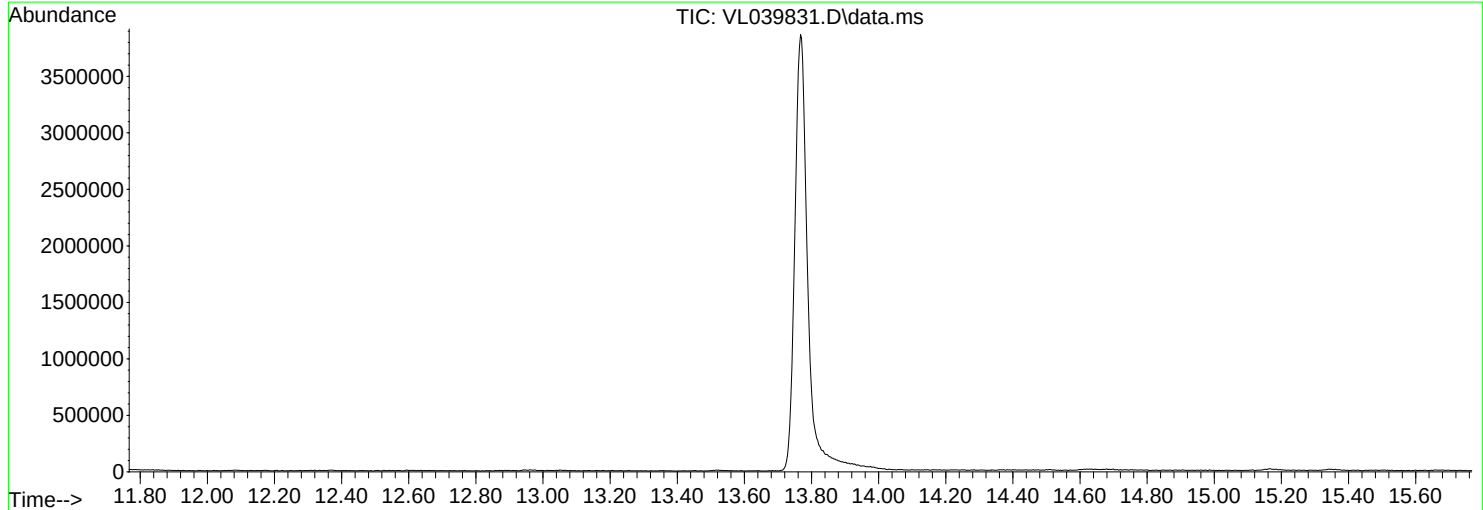

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.7	184469	PASS
75	95	30	66	52.9	449003	PASS
95	95	100	100	100.0	848747	PASS
96	95	5	9	7.1	60501	PASS
173	174	0.00	2	0.8	4341	PASS
174	95	50	120	63.1	535253	PASS
175	174	4	9	7.5	40232	PASS
176	174	93	101	95.4	510848	PASS
177	176	5	9	6.6	33957	PASS

Average of 13.764 to 13.770 min.: VL039831.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	2237	45.05	6375	56.05	11617	65.10	191
36.15	4304	46.15	455	57.05	24237	65.30	17
37.05	40139	47.05	8666	57.90	617	67.00	177
38.05	39509	47.85	2521	58.20	488	68.10	9628
39.10	15076	48.05	2866	58.70	115	69.05	94629
40.00	807	49.05	32968	59.00	62	70.05	7004
41.15	270	50.10	184469	60.05	6832	70.90	145
42.95	334	51.05	56589	61.00	37088	72.00	3229
43.20	223	52.10	2269	62.05	38395	73.05	32701
44.00	4967	52.90	236	63.10	29144	74.10	149973
44.90	2824	55.05	1782	64.05	2950	75.10	449003

Average of 13.764 to 13.770 min.: VL039831.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.10	38576	86.00	697	101.60	82	112.95	626
77.05	3838	87.05	27411	102.85	396	114.75	555
78.00	2617	88.00	26709	104.00	3536	115.00	335
78.95	21181	90.20	188	105.05	835	116.05	2426
80.05	5210	90.95	2762	105.95	3407	116.95	4296
81.00	20773	92.10	22949	106.90	991	118.05	2879
81.90	4289	93.05	35568	109.80	448	118.95	4214
82.80	153	94.10	98613	110.90	823	120.00	141
83.25	495	95.10	848747	111.60	56	121.90	183
85.40	101	96.10	60501	112.05	431	122.95	135
85.70	110	97.05	1932	112.70	346	123.85	657

Average of 13.764 to 13.770 min.: VL039831.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.80	250	135.00	1247	143.90	538	155.00	2143
125.95	372	136.00	207	144.95	746	155.95	157
126.60	55	136.90	820	145.95	902	157.05	1327
126.90	58	138.95	294	146.95	684	159.10	809
127.20	174	139.85	212	148.00	1814	160.95	919
128.00	3165	140.10	206	149.05	724	161.80	51
129.00	1070	141.00	5966	149.70	249	162.90	85
130.05	3116	141.70	278	150.10	374	166.20	68
130.80	434	142.00	470	151.90	370	167.90	64
131.05	556	142.20	564	153.00	426	169.10	135
134.00	88	143.00	5630	154.05	551	169.40	169

Average of 13.764 to 13.770 min.: VL039831.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.00	229	189.80	56				
170.20	393	237.20	70				
170.70	451	278.20	85				
171.20	240	282.10	54				
171.90	1524						
173.00	4341						
174.10	535253						
175.05	40232						
176.10	510848						
177.05	33957						
178.10	1154						