
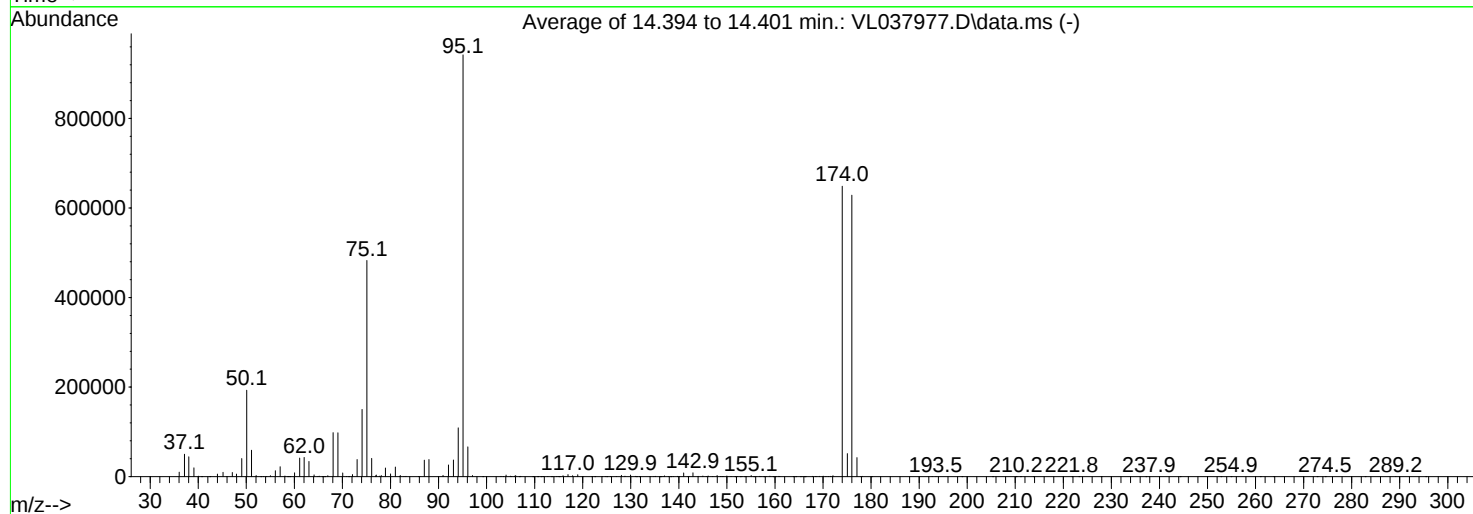


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110921\
 Data File : VL037977.D
 Acq On : 9 Nov 2021 8:18
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110121AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Nov 02 05:54:07 2021
 Last Update : Tue Nov 02 05:54:07 2021

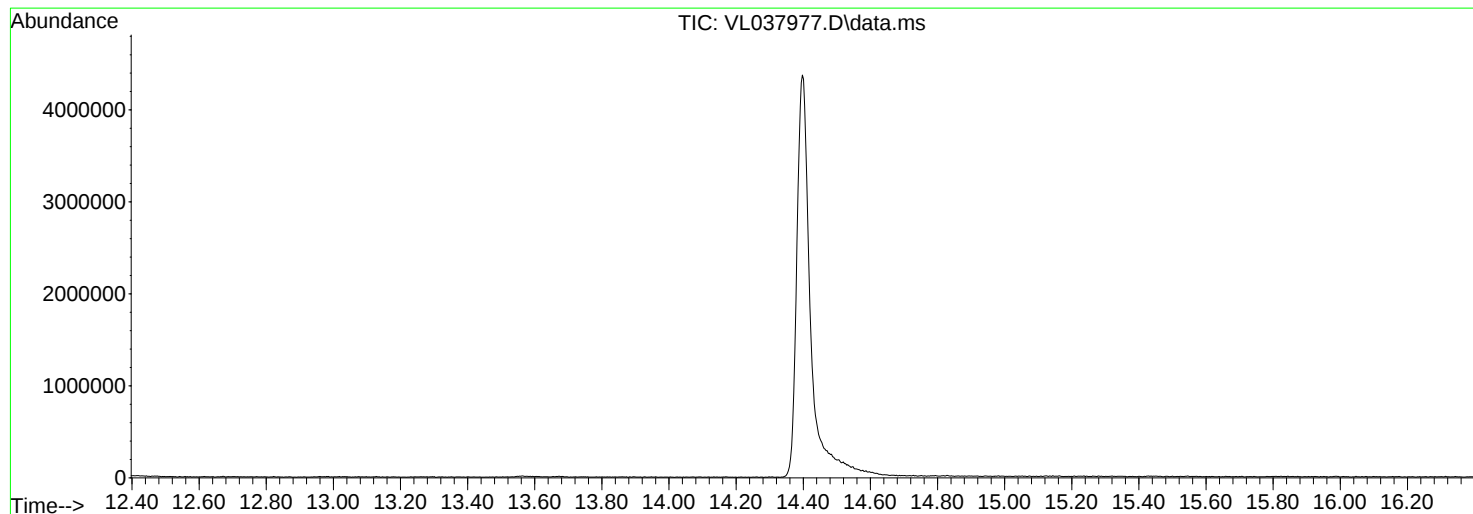

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.5	193024	PASS
75	95	30	66	51.3	482987	PASS
95	95	100	100	100.0	942123	PASS
96	95	5	9	7.0	66368	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.8	648512	PASS
175	174	4	9	7.9	51392	PASS
176	174	93	101	96.9	628565	PASS
177	176	5	9	6.8	42701	PASS

Average of 14.394 to 14.401 min.: VL037977.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	10135	47.95	5750	58.05	1468	66.05	40
37.15	50056	49.05	40381	58.60	130	66.30	7
38.05	44483	50.10	193024	59.00	125	66.95	202
39.10	19704	51.10	58925	60.05	8668	68.05	9813
40.10	1163	52.05	2640	61.10	41576	69.05	98061
40.70	121	53.00	133	62.05	42771	70.05	8236
42.40	52	53.60	285	63.05	33832	70.85	412
44.00	5795	54.25	211	64.10	3877	71.30	158
45.15	9626	55.00	2077	64.90	347	72.10	4679
45.95	478	56.05	13289	65.15	1042	73.05	38288
47.10	9468	57.05	22115	65.80	67	74.10	150101

Average of 14.394 to 14.401 min.: VL037977.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	482987	82.80	294	96.10	66368	107.10	856
76.10	40691	83.20	799	97.05	2483	109.60	80
76.90	1807	85.85	316	99.20	164	109.85	286
77.05	3603	86.10	507	103.00	592	110.60	100
77.70	1080	87.05	36715	103.50	367	110.85	554
78.10	2717	88.00	38400	104.05	3706	111.30	128
78.95	19362	90.95	2968	104.95	993	111.70	267
80.00	5930	92.05	26029	105.20	483	111.85	489
81.00	21483	93.10	37365	105.80	1138	112.75	446
81.90	892	94.10	109117	106.05	2474	113.50	155
82.05	2366	95.10	942123	106.80	111	114.60	326

Average of 14.394 to 14.401 min.: VL037977.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.90	523	125.00	154	134.80	525	141.00	8351
115.10	133	125.80	268	135.10	596	141.90	432
115.90	2014	127.00	367	136.00	94	142.10	894
116.95	4635	128.05	2786	136.20	93	142.95	8691
117.90	2226	128.80	1103	136.70	328	144.00	634
118.95	4299	129.95	3737	137.00	1821	145.00	1510
119.90	72	130.95	914	137.80	198	145.70	204
121.90	120	131.20	152	138.30	87	146.10	1285
122.50	109	131.80	60	138.85	569	147.05	568
124.05	474	132.00	204	139.75	662	147.95	2361
124.70	192	134.00	279	140.10	305	148.70	238

Average of 14.394 to 14.401 min.: VL037977.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.00	379	155.60	125	163.80	108	170.60	463
149.20	246	156.05	232	164.30	140	171.10	470
150.00	1387	156.85	790	165.30	95	171.60	866
150.85	259	157.10	560	165.80	355	172.05	2305
151.70	76	157.70	80	166.10	63	174.00	648512
152.15	508	158.15	249	166.30	100	175.05	51392
152.80	54	158.95	1266	167.80	596	176.00	628565
153.15	490	159.60	82	168.45	334	177.05	42701
153.70	180	160.05	169	168.70	300	177.85	331
154.10	460	160.80	679	169.25	608	178.15	791
155.05	2471	161.00	234	170.05	979	180.10	106

Average of 14.394 to 14.401 min.: VL037977.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
192.70	255	237.90	216				
193.50	260	244.30	102				
198.90	103	252.80	52				
205.30	58	254.90	134				
210.20	78	261.00	80				
211.10	105	263.80	70				
213.80	51	272.80	77				

221.80	166	274.50	169
223.25	150	282.80	97
227.85	132	289.20	280
237.20	177	295.40	50

Instrument :
MSVOA_L
ClientSampleId :
BFB