

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL111220\  
 Data File : VL035921.D  
 Acq On : 12 Nov 2020 20:01  
 Operator : SY/AP  
 Sample : L4720-05  
 Misc : 400ml/MSVOA L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 CVS-5

## Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON  
 Sampling : 3  
 Start Thrs: 0.001  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Wed Nov 04 02:40:06 2020

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.864       | 11            | 24          | 56           | rBV      | 2849457        | 6699755       | 53.33%          | 9.552%        |
| 2         | 3.012       | 62            | 70          | 77           | rBV3     | 120455         | 197520        | 1.57%           | 0.282%        |
| 3         | 3.195       | 117           | 127         | 142          | rBV      | 210971         | 339068        | 2.70%           | 0.483%        |
| 4         | 3.346       | 165           | 174         | 187          | rBV      | 352777         | 531141        | 4.23%           | 0.757%        |
| 5         | 3.597       | 241           | 252         | 268          | rBV      | 302319         | 713270        | 5.68%           | 1.017%        |
| 6         | 3.864       | 319           | 335         | 351          | rBV2     | 568744         | 1500560       | 11.94%          | 2.139%        |
| 7         | 3.967       | 351           | 367         | 373          | rVV2     | 124278         | 373345        | 2.97%           | 0.532%        |
| 8         | 4.121       | 406           | 415         | 429          | rBV      | 237025         | 397103        | 3.16%           | 0.566%        |
| 9         | 4.337       | 461           | 482         | 518          | rBV      | 2087655        | 4427055       | 35.24%          | 6.312%        |
| 10        | 5.054       | 691           | 705         | 712          | rBV3     | 97400          | 191639        | 1.53%           | 0.273%        |
| 11        | 5.102       | 712           | 720         | 732          | rVV3     | 189035         | 373961        | 2.98%           | 0.533%        |
| 12        | 5.366       | 788           | 802         | 819          | rBV4     | 111341         | 229330        | 1.83%           | 0.327%        |
| 13        | 5.671       | 876           | 897         | 938          | rBV2     | 3524235        | 10540989      | 83.91%          | 15.028%       |
| 14        | 6.314       | 1083          | 1097        | 1117         | rBV6     | 112866         | 324581        | 2.58%           | 0.463%        |
| 15        | 6.886       | 1262          | 1275        | 1287         | rBV3     | 82211          | 166040        | 1.32%           | 0.237%        |
| 16        | 7.169       | 1336          | 1363        | 1382         | rBV2     | 4478833        | 9681746       | 77.07%          | 13.803%       |
| 17        | 7.247       | 1386          | 1387        | 1403         | rVV5     | 163465         | 233420        | 1.86%           | 0.333%        |
| 18        | 7.481       | 1441          | 1460        | 1476         | rBV6     | 123254         | 302279        | 2.41%           | 0.431%        |
| 19        | 7.867       | 1564          | 1580        | 1606         | rVB      | 196034         | 501070        | 3.99%           | 0.714%        |
| 20        | 8.121       | 1646          | 1659        | 1670         | rBV6     | 78134          | 168213        | 1.34%           | 0.240%        |
| 21        | 8.812       | 1862          | 1874        | 1897         | rVB7     | 64331          | 163009        | 1.30%           | 0.232%        |
| 22        | 9.803       | 2163          | 2182        | 2208         | rBV      | 2101226        | 4457245       | 35.48%          | 6.355%        |
| 23        | 10.433      | 2364          | 2378        | 2388         | rBV6     | 49679          | 133592        | 1.06%           | 0.190%        |
| 24        | 11.697      | 2755          | 2771        | 2791         | rVB      | 92091          | 245549        | 1.95%           | 0.350%        |
| 25        | 12.086      | 2870          | 2892        | 2926         | rBV      | 4963386        | 11701103      | 93.14%          | 16.682%       |
| 26        | 12.967      | 3151          | 3166        | 3188         | rBV4     | 114032         | 383115        | 3.05%           | 0.546%        |
| 27        | 14.417      | 3599          | 3617        | 3659         | rBV      | 5179197        | 12562913      | 100.00%         | 17.911%       |
| 28        | 16.121      | 4132          | 4147        | 4168         | rVB5     | 78134          | 223132        | 1.78%           | 0.318%        |
| 29        | 16.773      | 4334          | 4350        | 4362         | rBV4     | 77872          | 188173        | 1.50%           | 0.268%        |
| 30        | 16.986      | 4398          | 4416        | 4442         | rBV      | 624649         | 1719871       | 13.69%          | 2.452%        |
| 31        | 17.114      | 4445          | 4456        | 4471         | rVB8     | 73634          | 187623        | 1.49%           | 0.267%        |
| 32        | 17.950      | 4696          | 4716        | 4730         | rBV8     | 92257          | 284029        | 2.26%           | 0.405%        |

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL111220\  
Data File : VL035921.D  
Acq On : 12 Nov 2020 20:01  
Operator : SY/AP  
Sample : L4720-05  
Misc : 400ml/MSVOA L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
CVS-5

Integration Parameters: RTEINT.P  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 3 Min Area: 3 % of largest Peak  
Start Thrs: 0.001 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL110320AIR.M  
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_LWed Nov 04 02:40:06 2020




Sum of corrected areas: 70141439

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL111220\  
Data File : VL035921.D  
Acq On : 12 Nov 2020 20:01  
Operator : SY/AP  
Sample : L4720-05  
Misc : 400ml/MSVOA L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
CVS-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M  
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_L Wed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

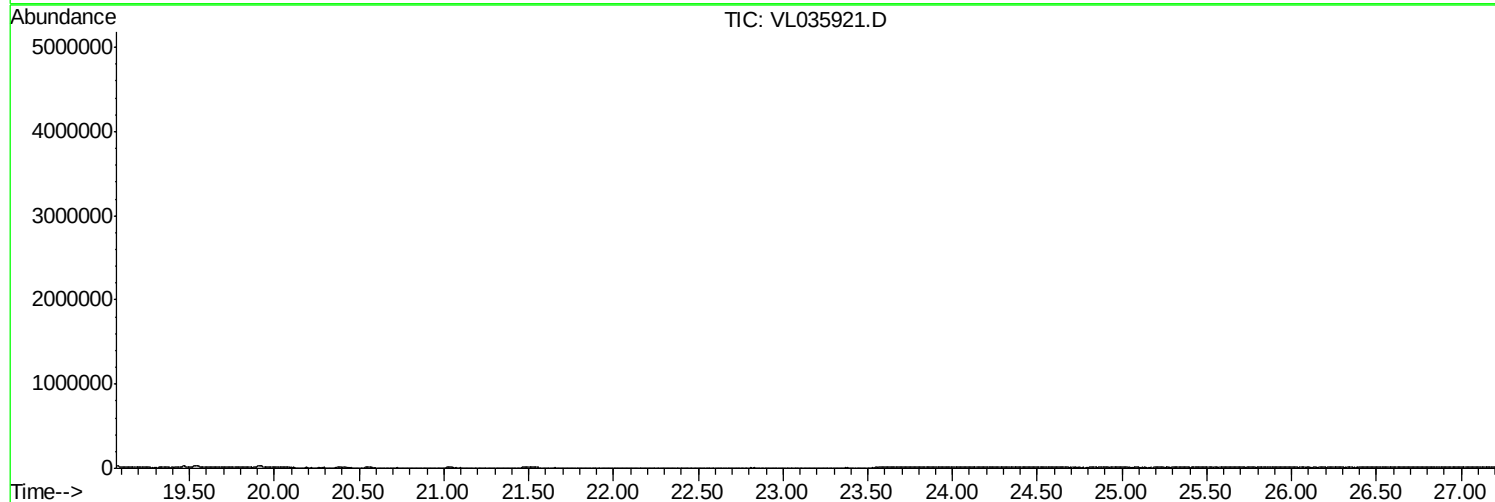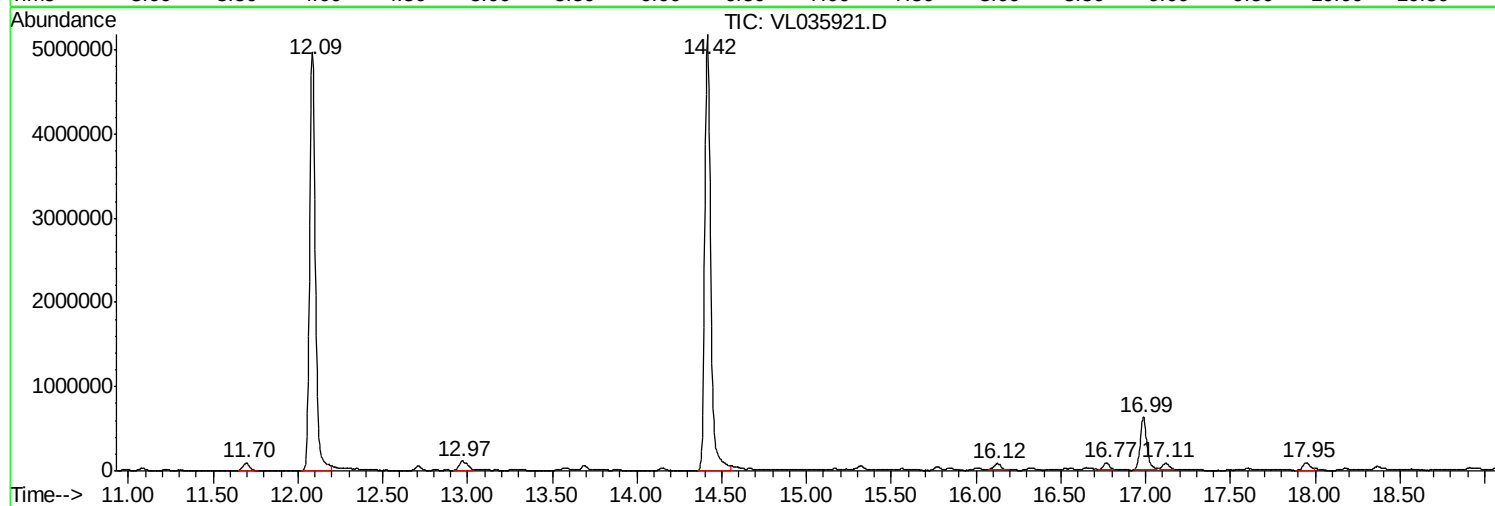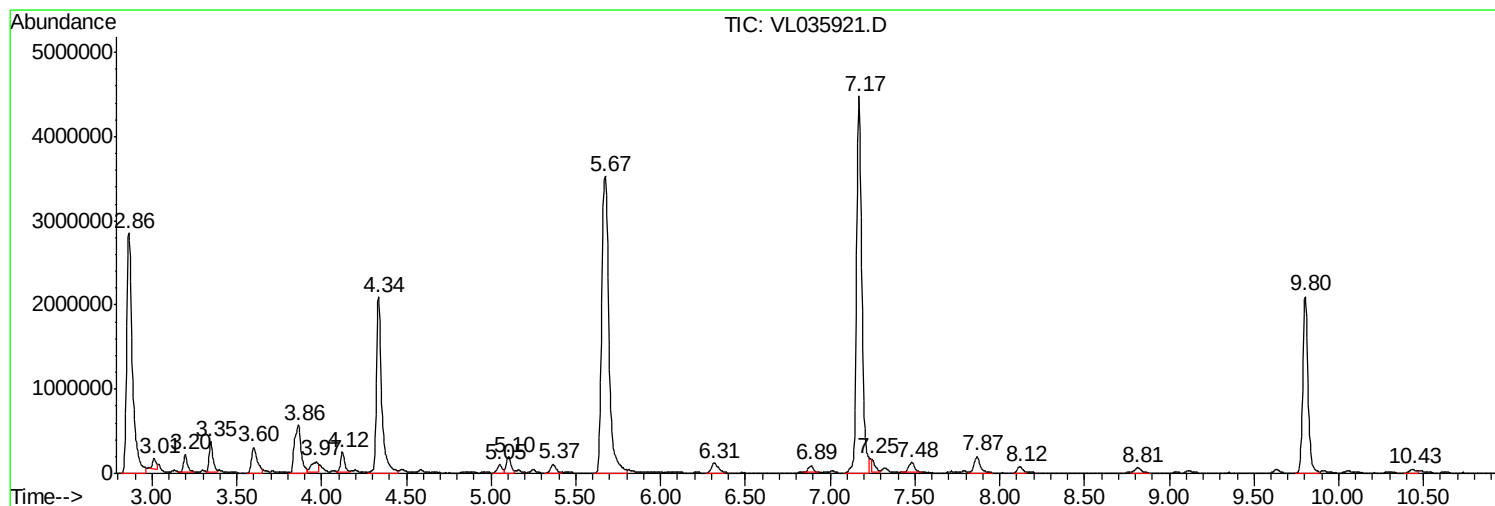

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_L\DATA\VL111220\  
Data File : VL035921.D  
Acq On : 12 Nov 2020 20:01  
Operator : SY/AP  
Sample : L4720-05  
Misc : 400ml/MSVOA\_L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
CVS-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_L\METHODS\VL110320AIR.M  
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_L\DATA\VL111220\  
Data File : VL035921.D  
Acq On : 12 Nov 2020 20:01  
Operator : SY/AP  
Sample : L4720-05  
Misc : 400ml/MSVOA\_L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
CVS-5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL110320AIR.M  
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |