


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL111220\
Data File : VL035907.D
Acq On : 12 Nov 2020 8:59
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020
Last Update : Wed Nov 04 02:40:06 2020

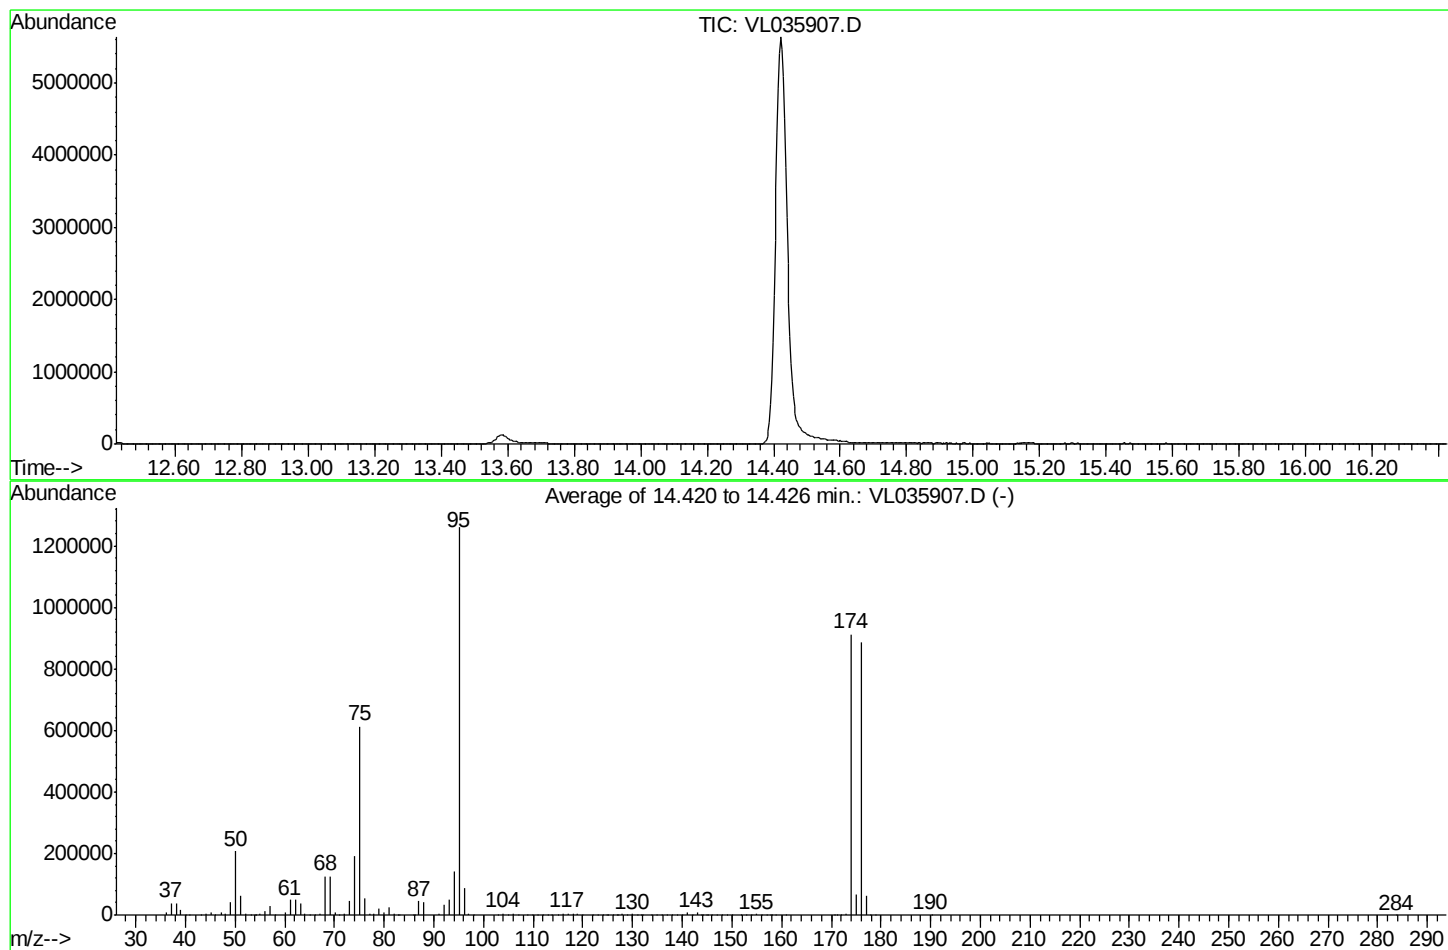

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	16.4	206698	PASS
75	95	30	66	48.7	613354	PASS
95	95	100	100	100.0	1260544	PASS
96	95	5	9	6.9	87002	PASS
173	174	0.00	2	0.5	4580	PASS
174	95	50	120	72.3	911850	PASS
175	174	4	9	7.3	66456	PASS
176	174	93	101	97.4	888256	PASS
177	176	5	9	6.9	60882	PASS