
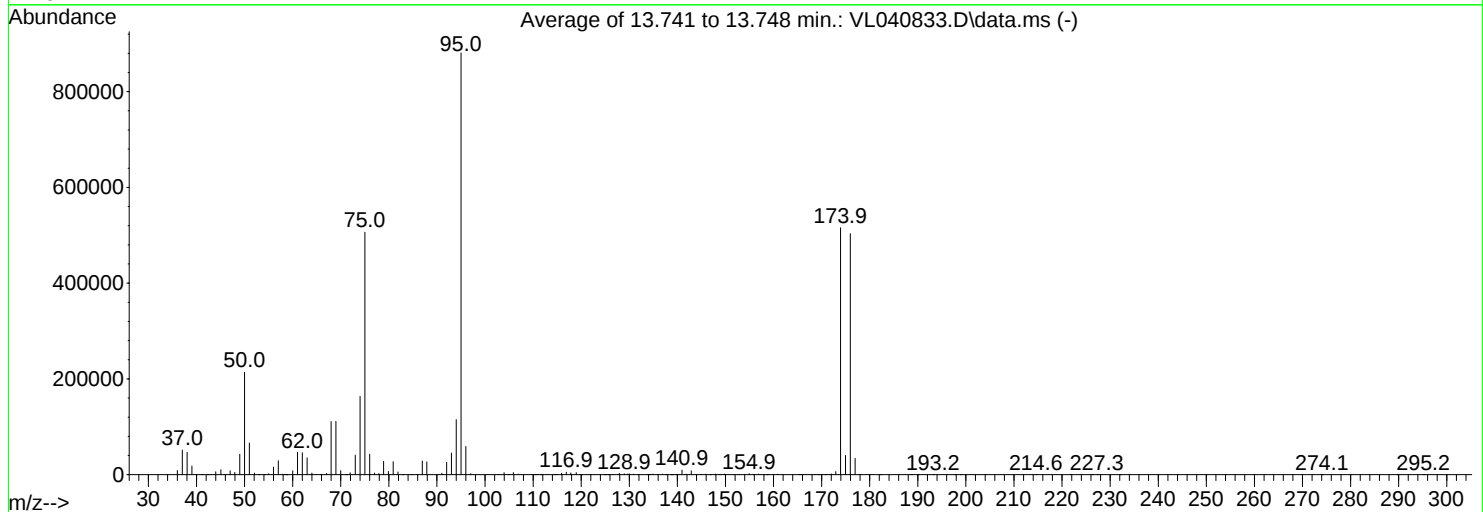


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111323\
Data File : VL040833.D
Acq On : 13 Nov 2023 9:29
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111323AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Nov 13 15:42:46 2023

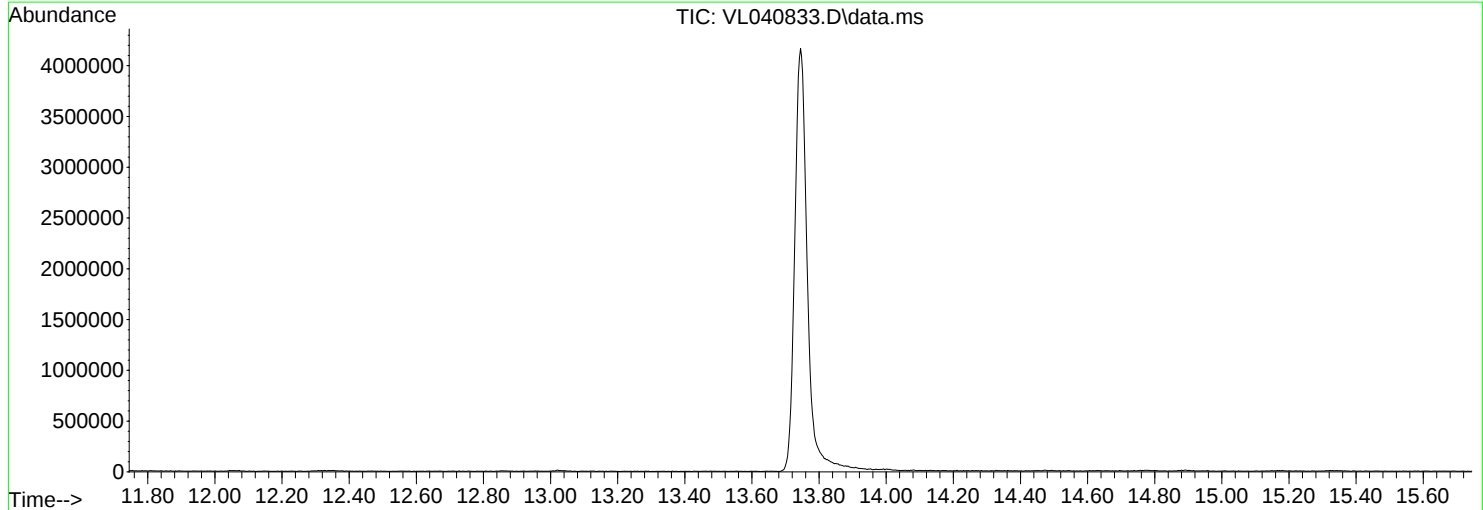

AutoFind: Scans 3464, 3465, 3466; Background Corrected with Scan 3438

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.3	213824	PASS
75	95	30	66	57.5	506325	PASS
95	95	100	100	100.0	881037	PASS
96	95	5	9	6.7	58973	PASS
173	174	0.00	2	1.3	6482	PASS
174	95	50	120	58.6	515861	PASS
175	174	4	9	7.8	40101	PASS
176	174	93	101	97.6	503275	PASS
177	176	5	9	6.8	34243	PASS

Average of 13.741 to 13.748 min.: VL040833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8591	47.00	8155	57.95	1074	67.05	2621
37.05	51645	47.95	4694	58.30	207	68.00	11097
38.05	46840	49.00	42363	58.60	116	69.00	11117
39.05	18063	50.00	213824	58.80	109	70.00	849
39.90	313	51.00	66315	60.00	8123	71.00	193
41.10	146	52.05	3301	61.00	46459	71.20	90
42.30	65	53.00	12	62.00	45800	71.95	3956
43.10	569	54.10	41	63.00	35125	73.00	40864
44.00	5909	55.00	1835	64.00	3371	74.00	163456
45.05	10310	56.00	15816	64.90	251	75.00	506325
45.90	640	57.00	29131	65.80	242	76.00	42856

Average of 13.741 to 13.748 min.: VL040833.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	3226	87.90	26857	105.10	306	114.90	651
77.95	2346	91.00	3189	105.90	4290	115.10	277
78.90	27824	92.00	25701	106.90	982	115.90	3129
79.90	6779	93.00	45219	109.80	370	116.90	5172
80.90	26965	94.00	115037	110.00	181	117.85	3529
81.90	5773	95.00	881037				