


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL111418\
 Data File : VL032741.D
 Acq On : 14 Nov 2018 1:49
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111418AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 14 07:00:23 2018
 Last Update : Wed Nov 14 07:00:23 2018

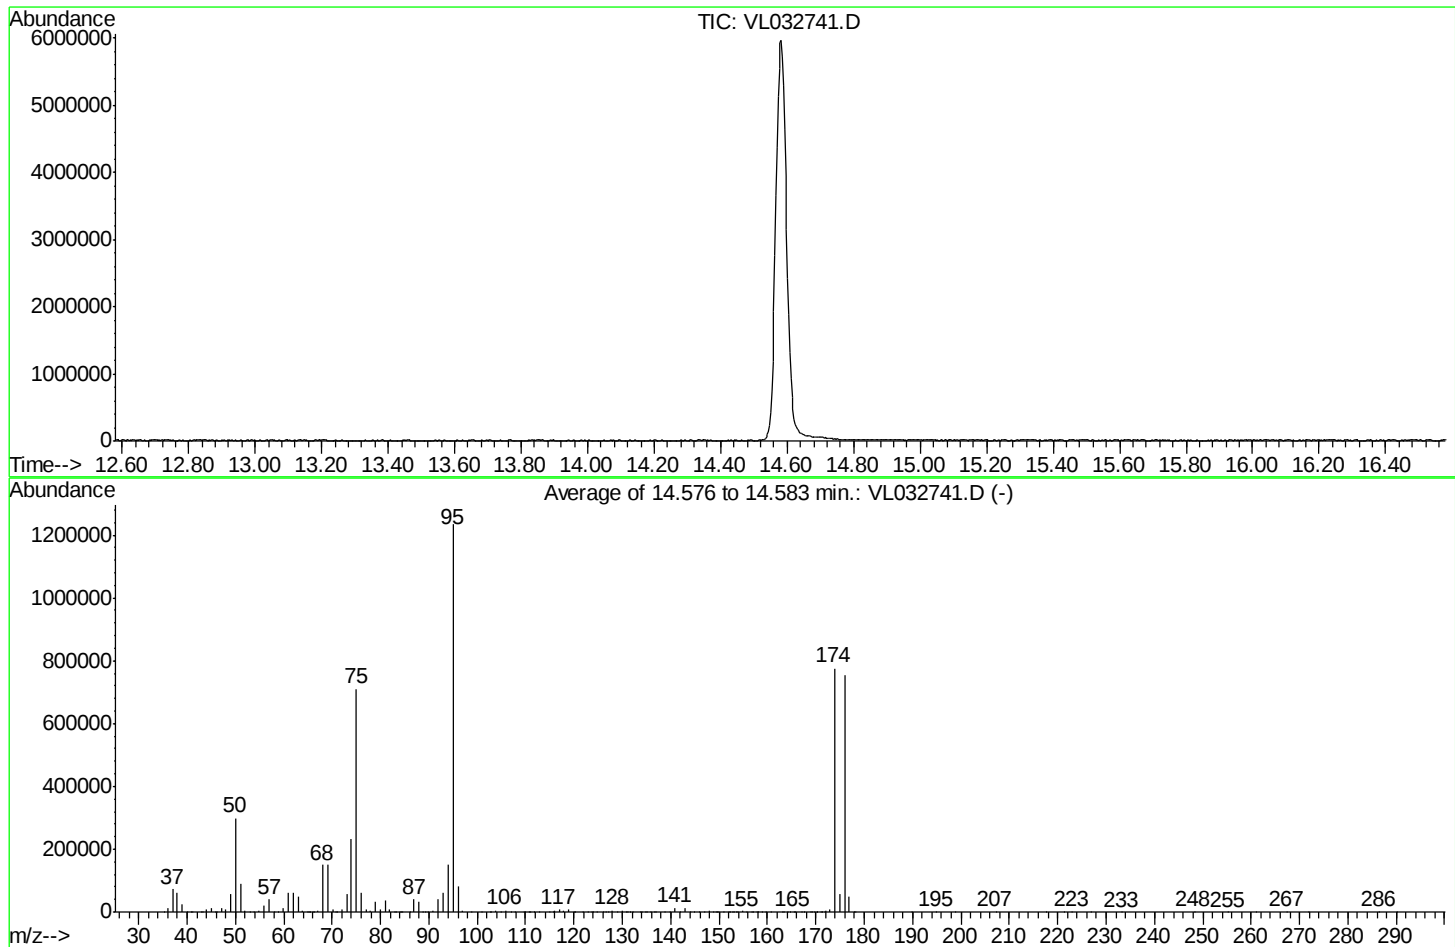

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	298133	PASS
75	95	30	66	57.5	709952	PASS
95	95	100	100	100.0	1234432	PASS
96	95	5	9	6.6	81482	PASS
173	174	0.00	2	1.2	9333	PASS
174	95	50	120	62.7	774528	PASS
175	174	4	9	7.6	58714	PASS
176	174	93	101	97.6	756117	PASS
177	176	5	9	6.7	50800	PASS