


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL111621\
 Data File : VL038022.D
 Acq On : 16 Nov 2021 1:08
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Nov 16 09:59:16 2021
 Last Update : Tue Nov 16 09:59:16 2021

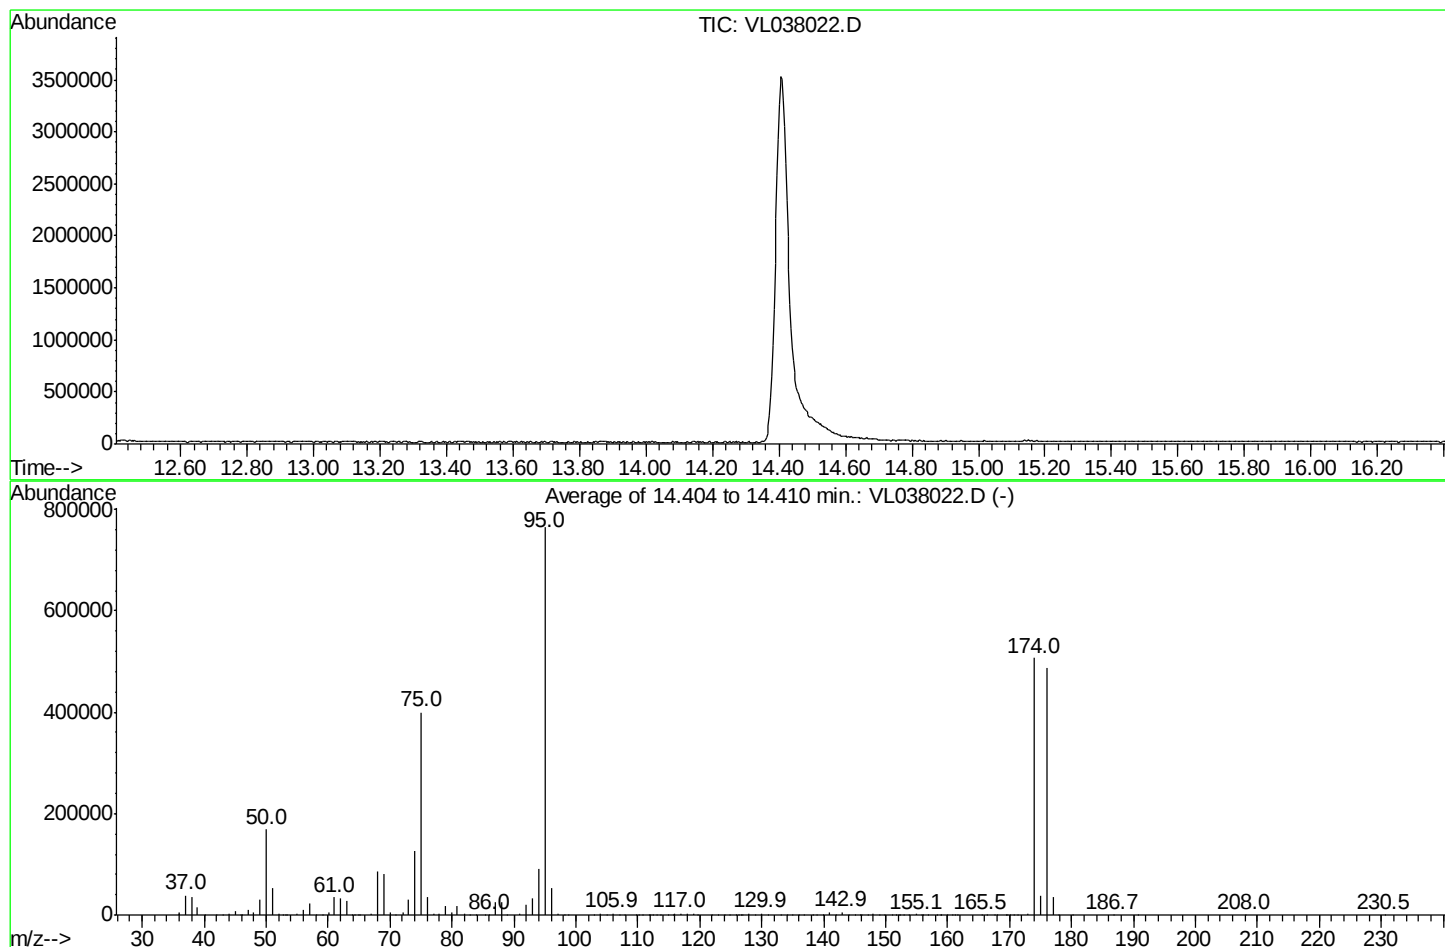

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.1	169183	PASS
75	95	30	66	52.3	400277	PASS
95	95	100	100	100.0	764864	PASS
96	95	5	9	6.8	52332	PASS
173	174	0.00	2	0.4	2232	PASS
174	95	50	120	66.3	507072	PASS
175	174	4	9	7.6	38749	PASS
176	174	93	101	96.4	488640	PASS
177	176	5	9	7.0	34298	PASS