


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_L\Data\VL111821\  
 Data File : VL038044.D  
 Acq On : 18 Nov 2021 7:32  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400mL/MSVOA\_L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL111821AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Tue Nov 16 09:59:16 2021  
 Last Update : Tue Nov 16 09:59:16 2021

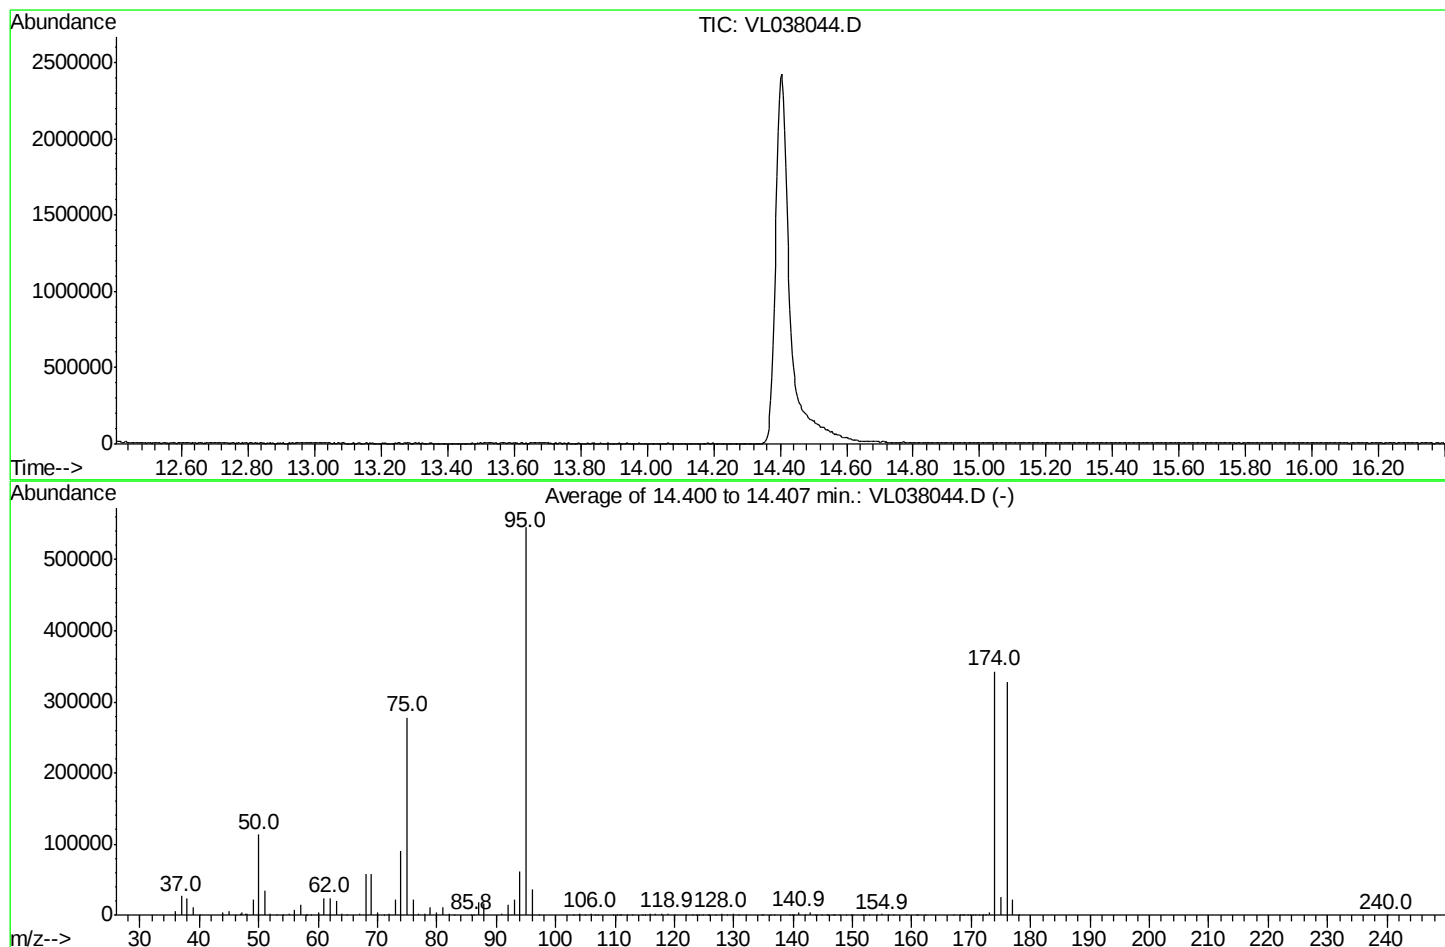

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3585

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 20.8      | 113389  | PASS             |
| 75          | 95           | 30           | 66           | 50.9      | 277802  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 545642  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 36549   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 4237    | PASS             |
| 174         | 95           | 50           | 120          | 62.8      | 342570  | PASS             |
| 175         | 174          | 4            | 9            | 7.4       | 25282   | PASS             |
| 176         | 174          | 93           | 101          | 95.7      | 327765  | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 22360   | PASS             |