


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL111921\
 Data File : VL038079.D
 Acq On : 19 Nov 2021 10:46
 Operator : SY/AP
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Nov 18 13:16:09 2021
 Last Update : Thu Nov 18 13:16:09 2021

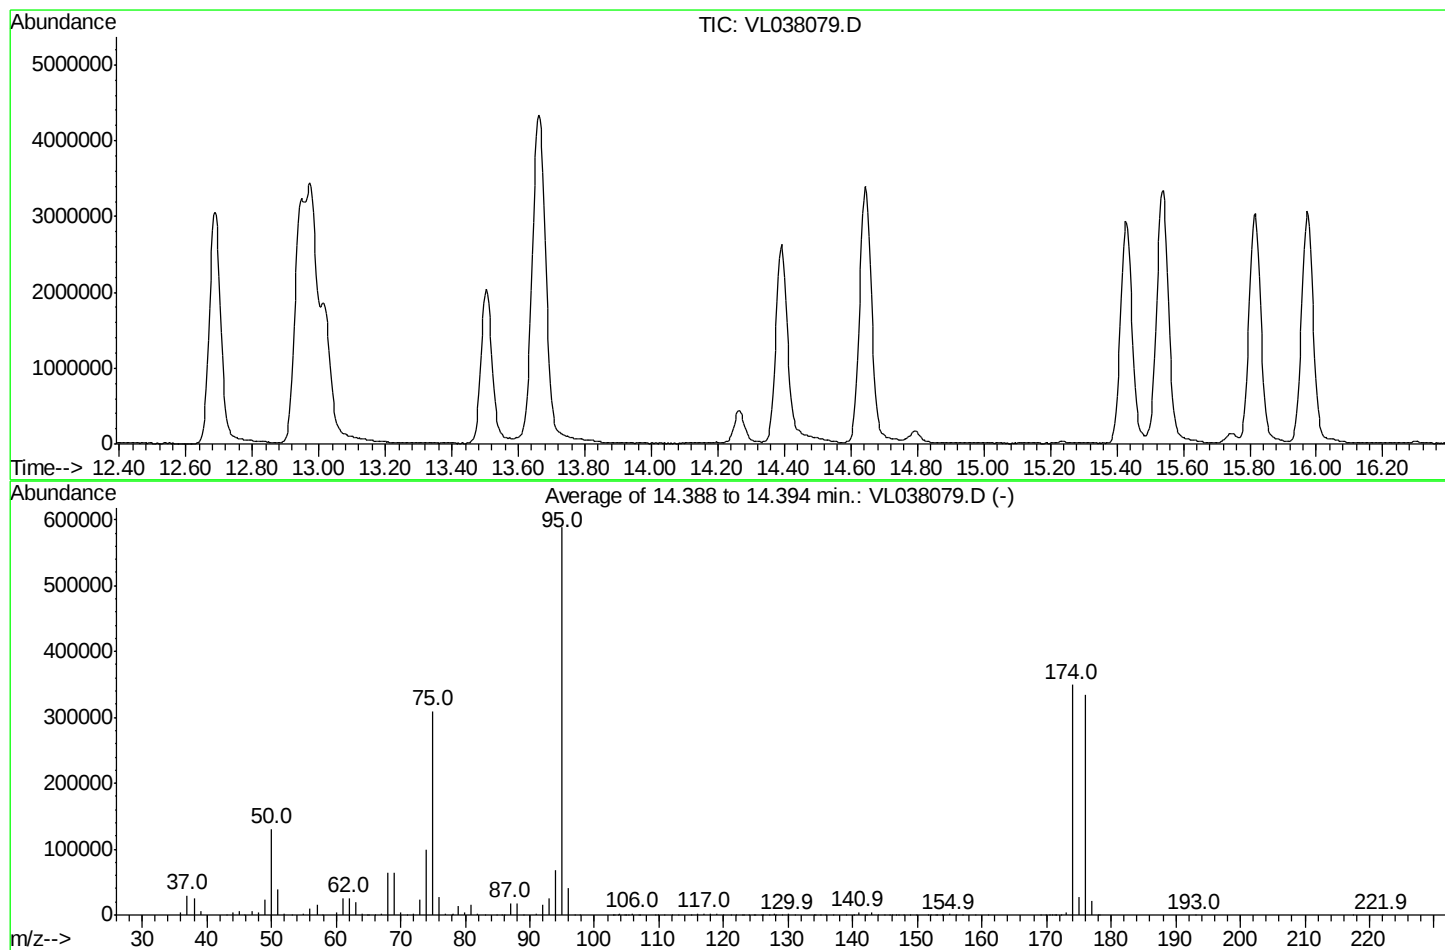

AutoFind: Scans 3608, 3609, 3610; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.2	130402	PASS
75	95	30	66	52.6	309696	PASS
95	95	100	100	100.0	588437	PASS
96	95	5	9	6.8	40146	PASS
173	174	0.00	2	1.1	3735	PASS
174	95	50	120	59.4	349418	PASS
175	174	4	9	7.5	26309	PASS
176	174	93	101	95.6	334186	PASS
177	176	5	9	6.7	22354	PASS