

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112222\
 Data File : VL039931.D
 Acq On : 23 Nov 2022 00:43
 Operator : SY/AP
 Sample : N5767-01DL 20X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV1DL

Quant Time: Nov 23 04:53:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Nov 22 03:45:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.176	49	971131	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	6.636	114	2713626	10.000	ppbv	0.02
55) Chlorobenzene-d5	11.455	117	2369554	10.000	ppbv	0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.767	95	1834726	10.137	ppbv	0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.400%
Target Compounds						
					Qvalue	
15) Acetone	3.465	43	43136	0.335	ppbv #	83
20) Methylene Chloride	3.912	84	22228	0.356	ppbv #	81
26) Hexane	5.195	57	75076	0.727	ppbv #	35
53) Toluene	9.208	91	47377	0.180	ppbv	100
74) 1,2,4-Trimethylbenzene	16.101	105	68158	0.244	ppbv #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112222\
Data File : VL039931.D
Acq On : 23 Nov 2022 00:43
Operator : SY/AP
Sample : N5767-01DL 20X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV1DL

Quant Time: Nov 23 04:53:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL11822AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Nov 22 03:45:31 2022
Response via : Initial Calibration




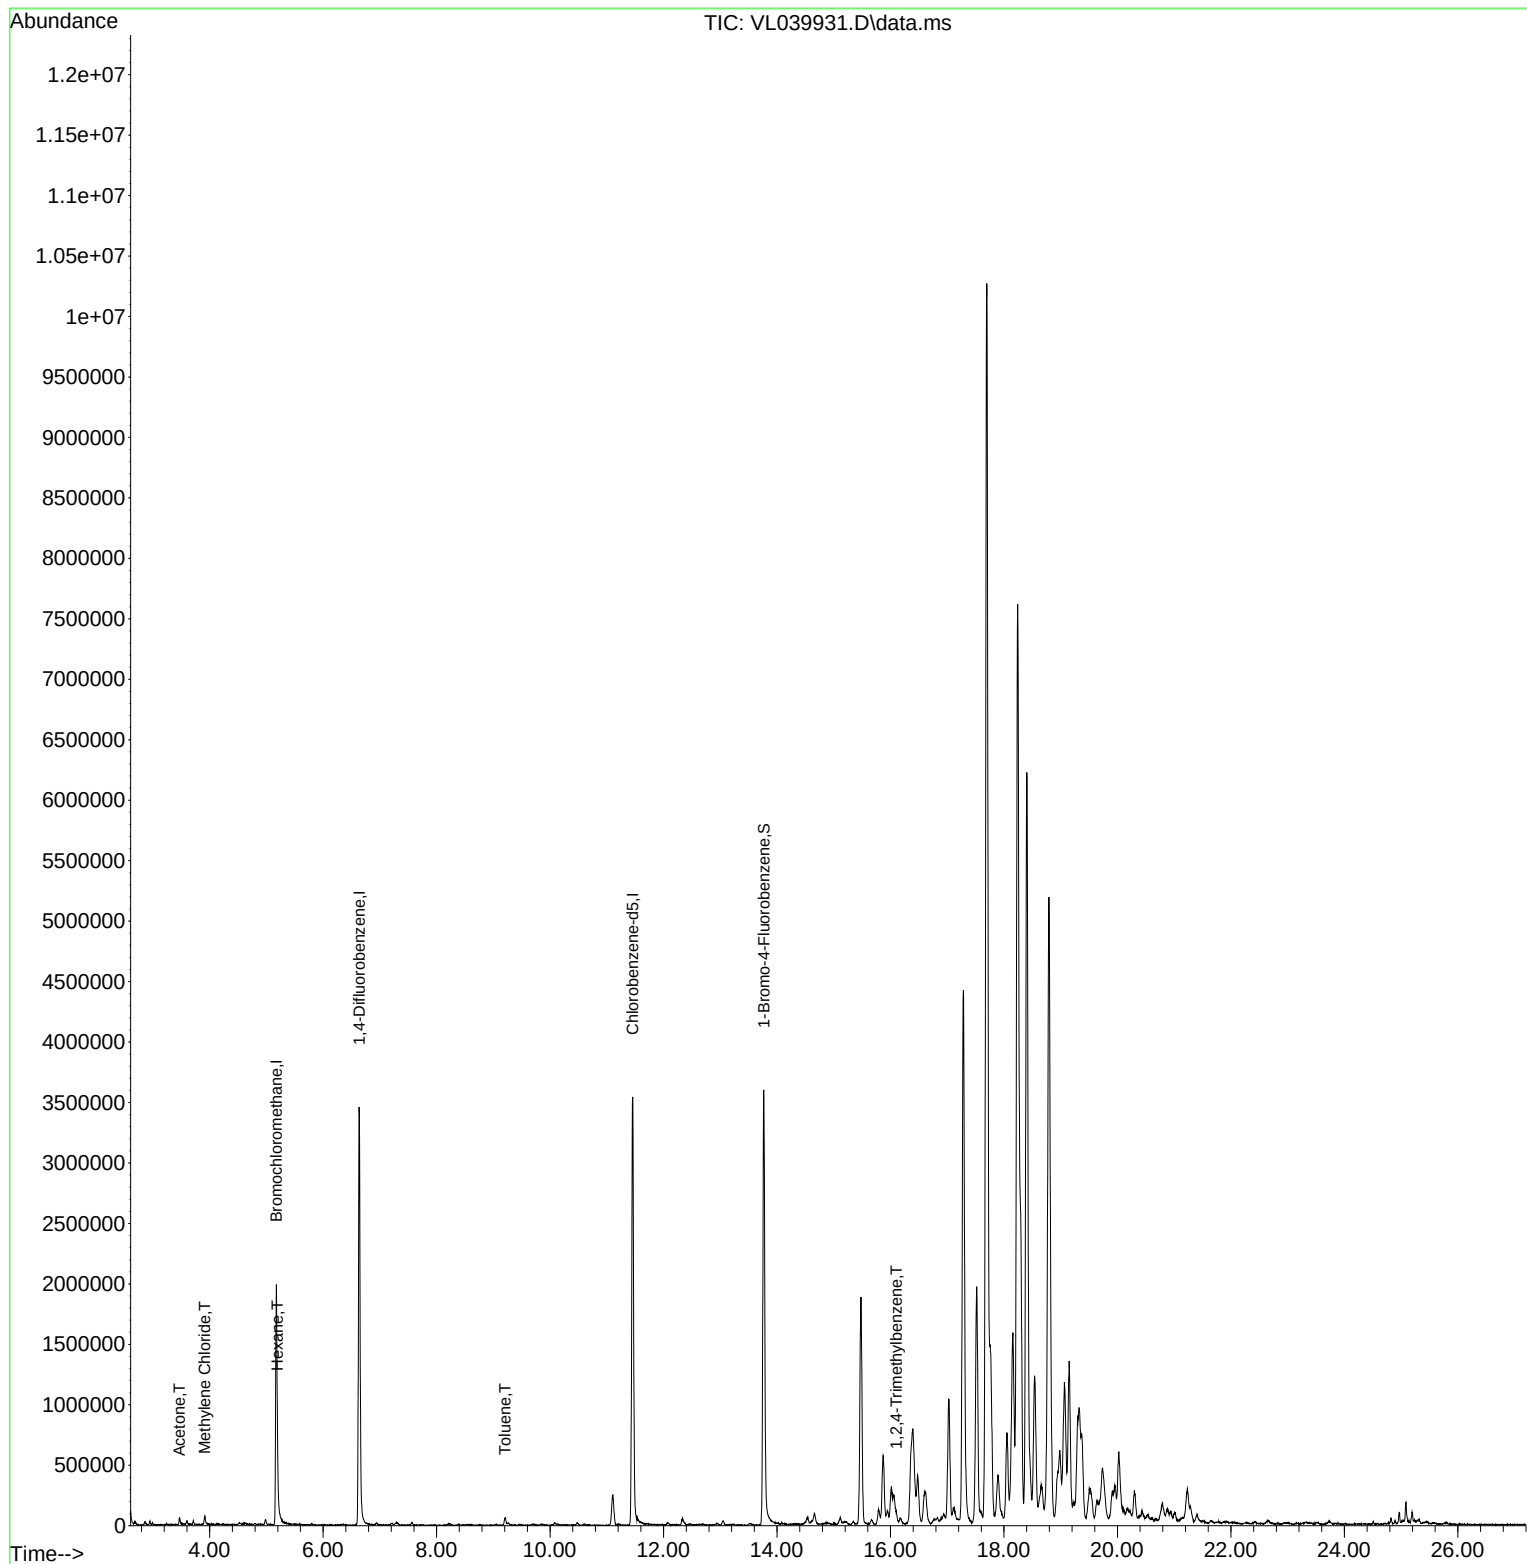


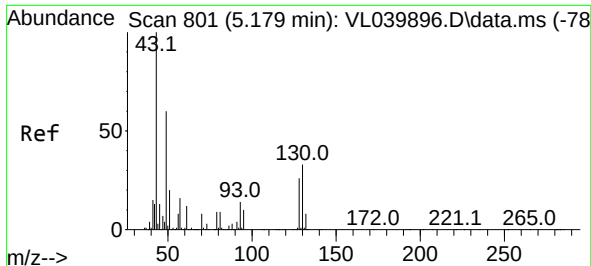

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.176 min Scan# 801
Delta R.T. 0.020 min
Lab File: VL039931.D
Acq: 23 Nov 2022 00:43




Instrument :
MSVOA_L
ClientSampleId :
SV1DL


Tgt Ion: 49 Resp: 971131
Ion Ratio Lower Upper
49 100
128 48.9 22.1 66.3
130 62.5 27.7 83.1

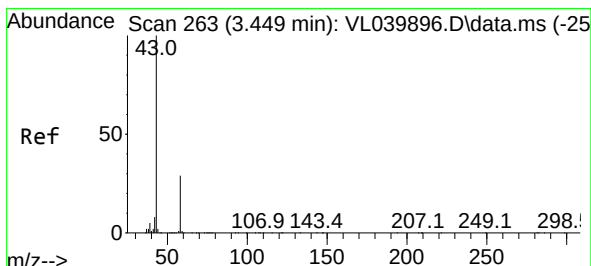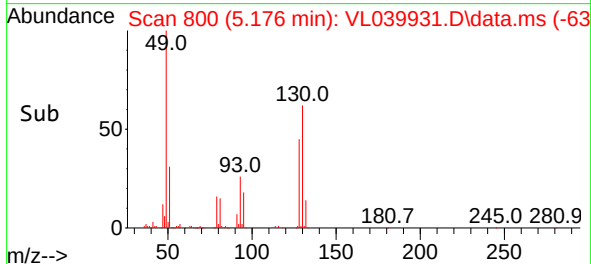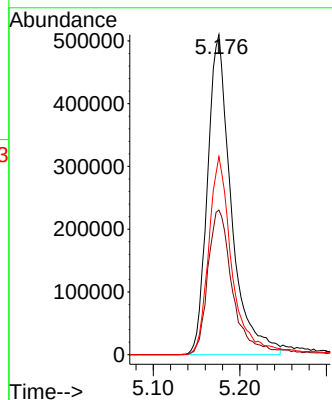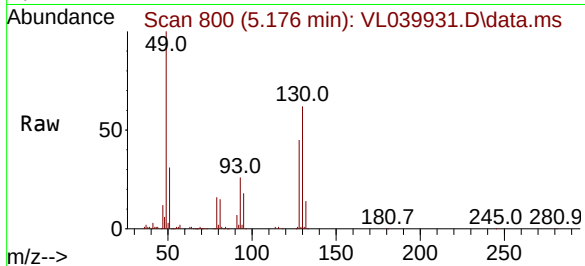

#15
Acetone
Concen: 0.335 ppbv
RT: 3.465 min Scan# 268
Delta R.T. 0.032 min
Lab File: VL039931.D
Acq: 23 Nov 2022 00:43

Tgt Ion: 43 Resp: 43136
Ion Ratio Lower Upper
43 100
58 37.5 22.9 34.3#


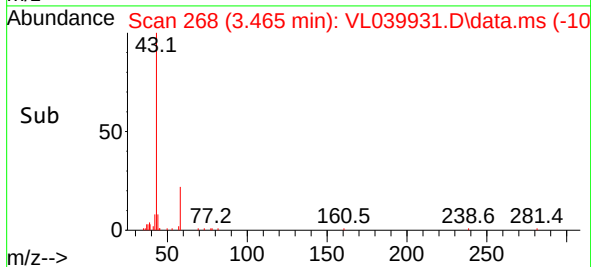
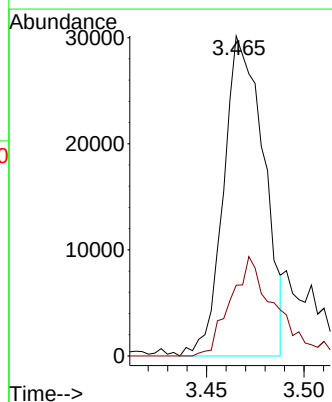
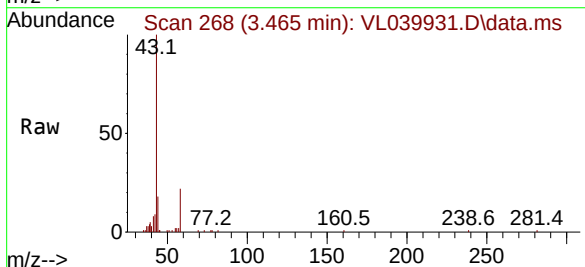


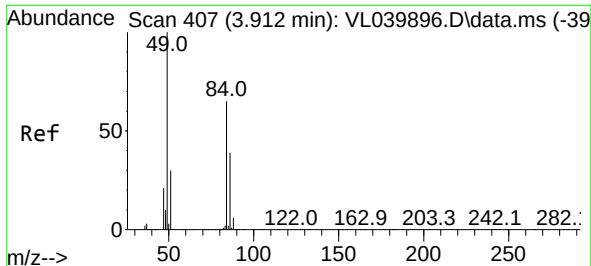

#20
Methylene Chloride
Concen: 0.356 ppbv
RT: 3.912 min Scan# 407
Delta R.T. 0.013 min
Lab File: VL039931.D
Acq: 23 Nov 2022 00:43




Instrument :
MSVOA_L
ClientSampleId :
SV1DL


Tgt Ion:	84	Resp:	22228
Ion	Ratio	Lower	Upper
84	100		
49	121.0	122.2	183.4#
51	31.6	36.3	54.5#
86	57.6	47.2	70.8

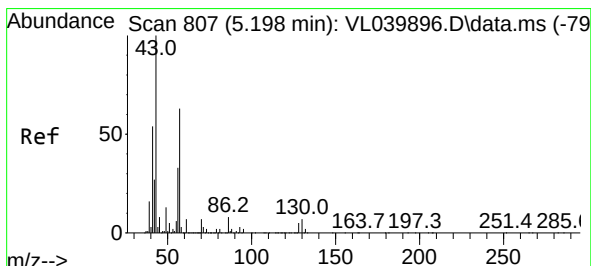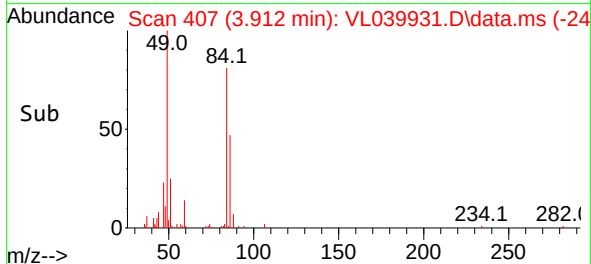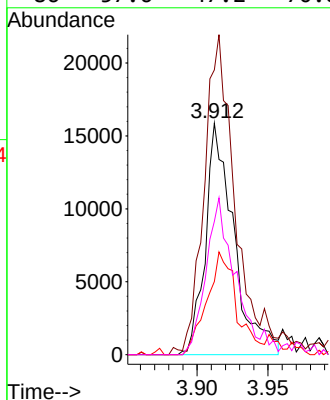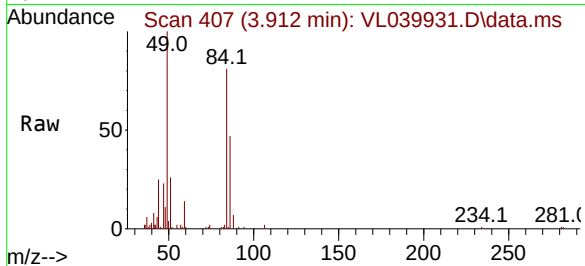

#26
Hexane
Concen: 0.727 ppbv
RT: 5.195 min Scan# 806
Delta R.T. 0.013 min
Lab File: VL039931.D
Acq: 23 Nov 2022 00:43

Tgt Ion:	57	Resp:	75076
Ion	Ratio	Lower	Upper
57	100		
41	107.8	72.3	108.5
43	74.1	188.7	283.1#
56	59.3	42.4	63.6

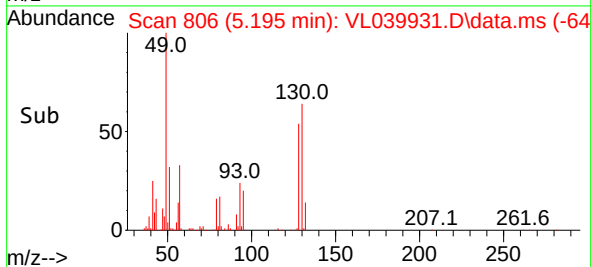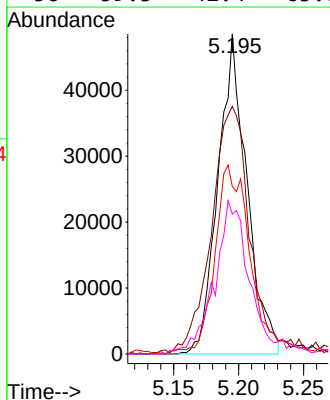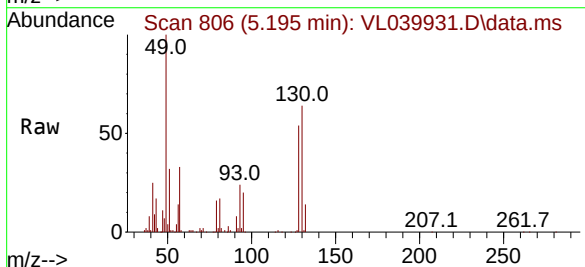

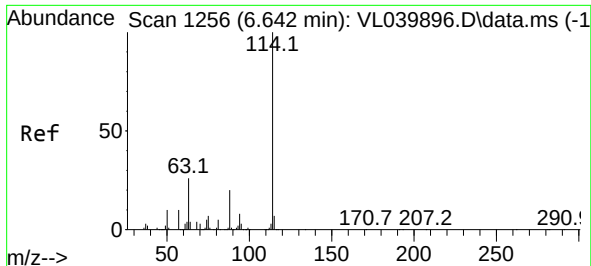

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.636 min Scan# 114

Delta R.T. 0.016 min

Lab File: VL039931.D

Acq: 23 Nov 2022 00:43

Instrument :

MSVOA_L

ClientSampleId :

SV1DL





Tgt Ion:114 Resp: 2713626

Ion Ratio Lower Upper

114 100

63 25.1 21.4 32.0

88 18.3 15.3 22.9

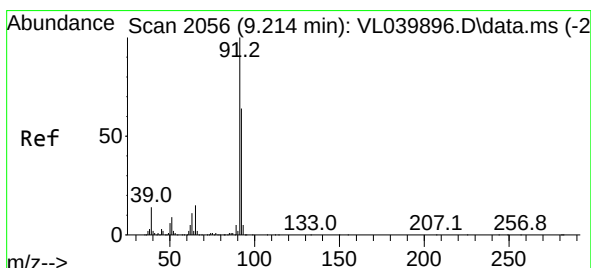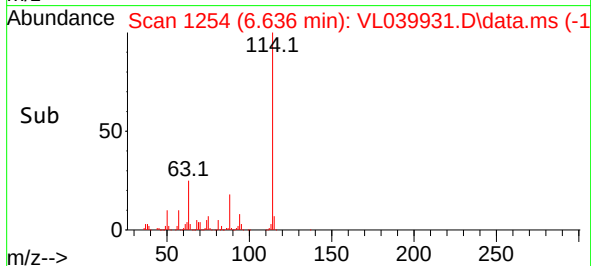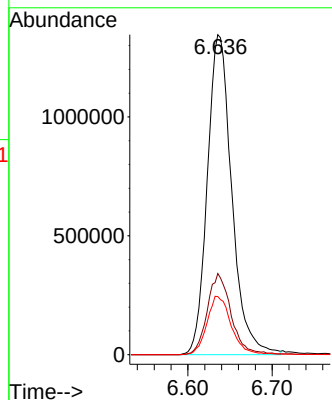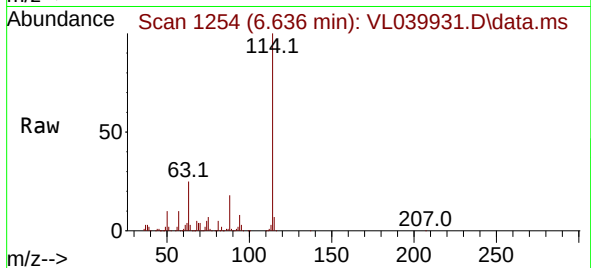

#53

Toluene

Concen: 0.180 ppbv

RT: 9.208 min Scan# 2054

Delta R.T. 0.016 min

Lab File: VL039931.D




Acq: 23 Nov 2022 00:43


Tgt Ion: 91 Resp: 47377

Ion Ratio Lower Upper

91 100

92 62.3 49.8 74.6


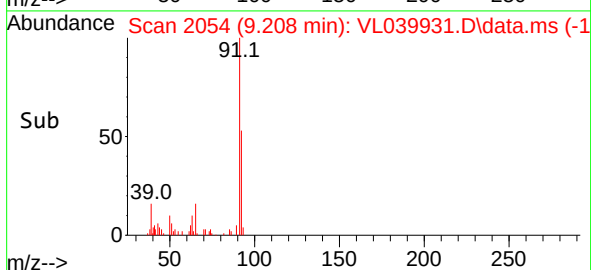
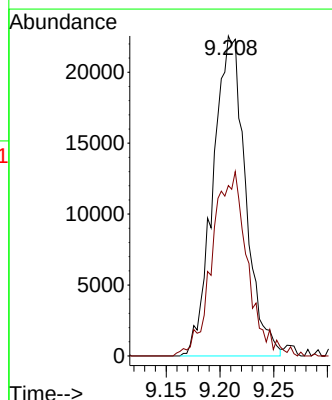
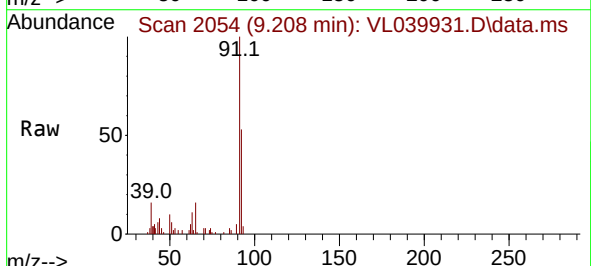


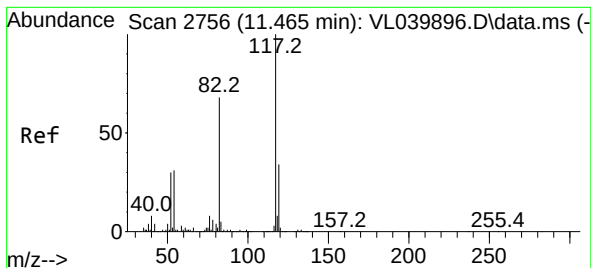

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.455 min Scan# 21
Delta R.T. 0.016 min
Lab File: VL039931.D
Acq: 23 Nov 2022 00:43




Instrument :
MSVOA_L
ClientSampleId :
SV1DL


Tgt Ion:117 Resp: 2369554
Ion Ratio Lower Upper
117 100
82 66.1 52.3 78.5
119 33.3 25.7 38.5

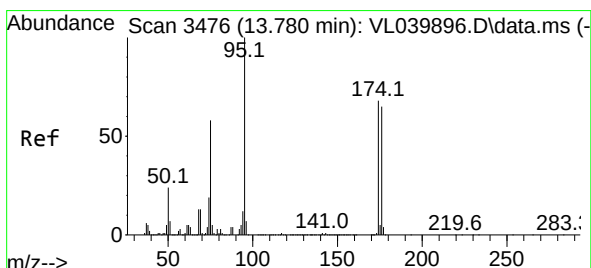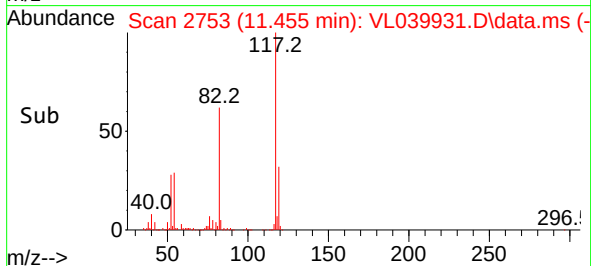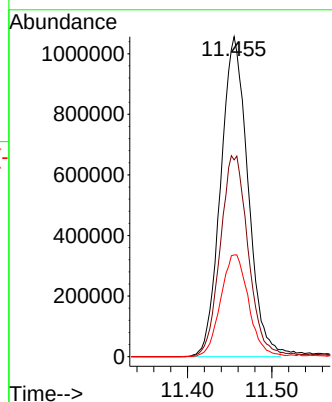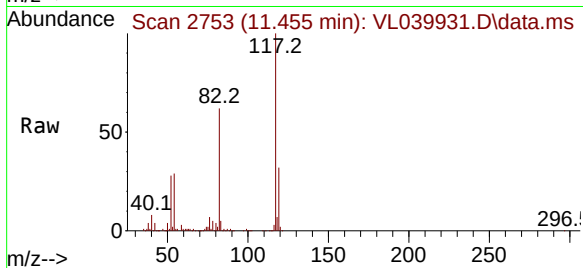

#68
1-Bromo-4-Fluorobenzene
Concen: 10.137 ppbv
RT: 13.767 min Scan# 3472
Delta R.T. 0.013 min
Lab File: VL039931.D
Acq: 23 Nov 2022 00:43

Tgt Ion: 95 Resp: 1834726
Ion Ratio Lower Upper
95 100
174 65.8 53.7 80.5
175 4.7 4.0 6.0

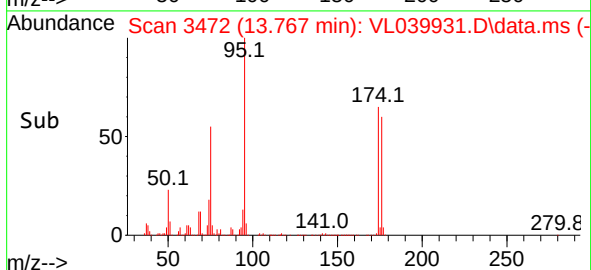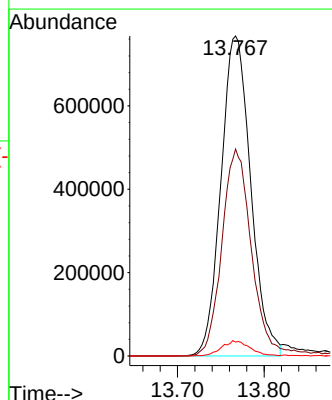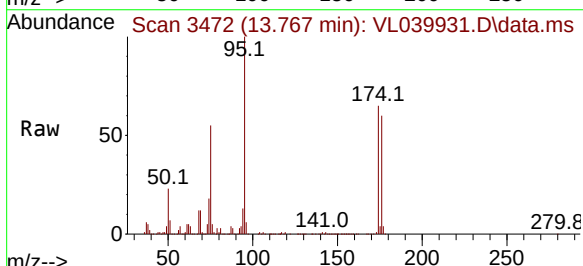

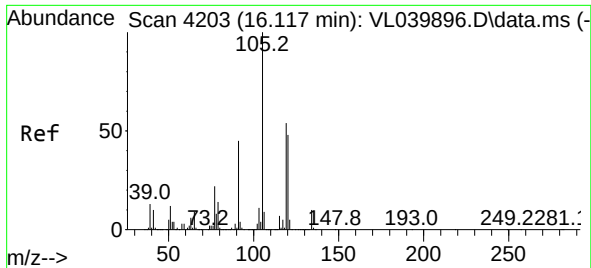

#74

1,2,4-Trimethylbenzene

Concen: 0.244 ppbv

RT: 16.101 min Scan# 41

Delta R.T. 0.010 min

Lab File: VL039931.D


Acq: 23 Nov 2022 00:43

Instrument :

MSVOA_L

ClientSampleId :

SV1DL

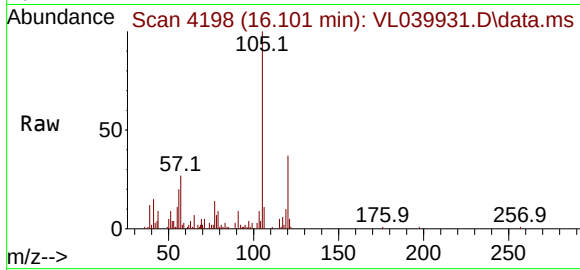

Tgt Ion:105 Resp: 68158

Ion Ratio Lower Upper

105 100

120 35.7 38.7 58.1#

91 9.2 36.4 54.6#

77 13.1 17.4 26.0#

