
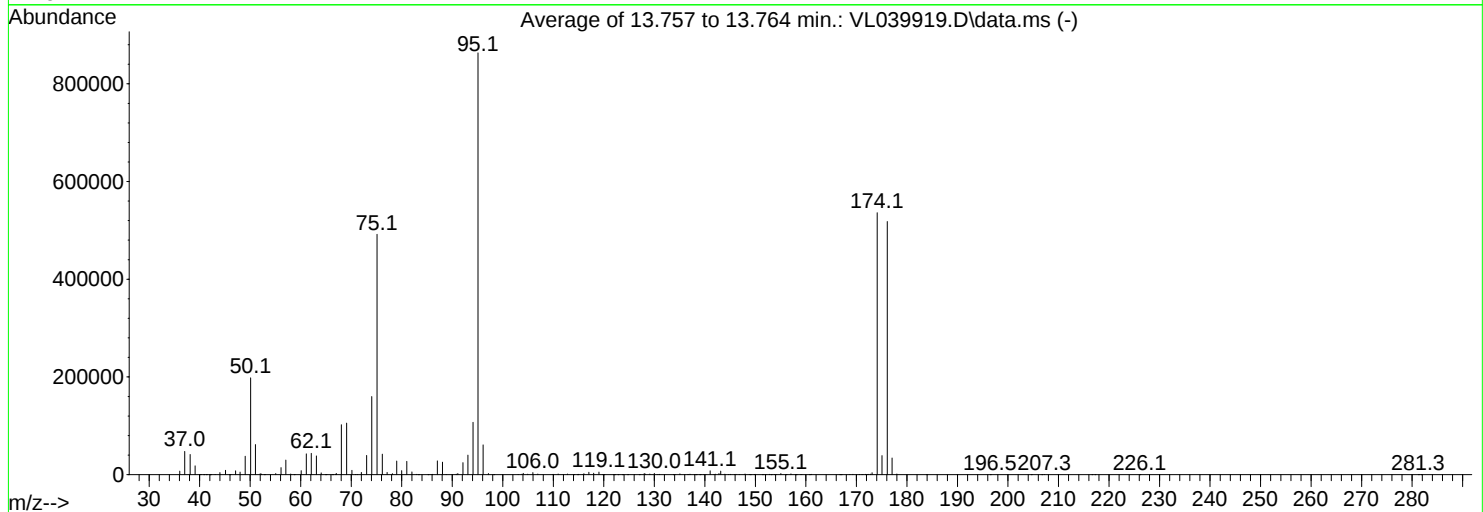


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112222\
Data File : VL039919.D
Acq On : 22 Nov 2022 15:42
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Nov 22 03:45:31 2022

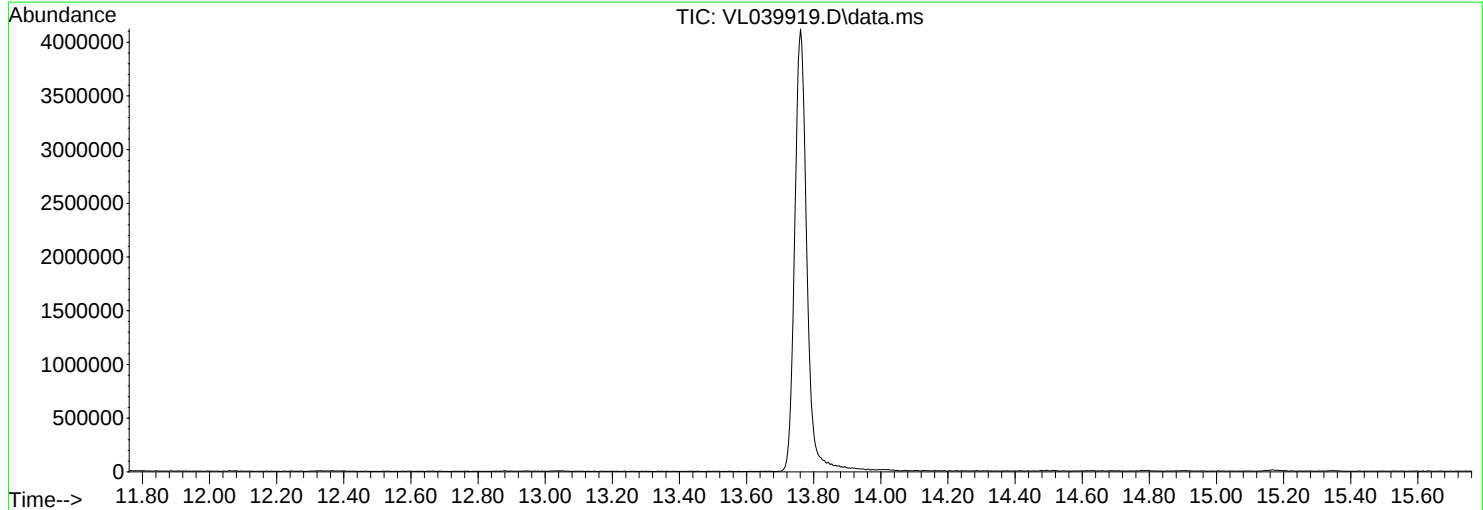

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	198229	PASS
75	95	30	66	57.0	491861	PASS
95	95	100	100	100.0	863403	PASS
96	95	5	9	7.1	60875	PASS
173	174	0.00	2	0.7	3845	PASS
174	95	50	120	62.1	536256	PASS
175	174	4	9	7.3	38992	PASS
176	174	93	101	96.6	518016	PASS
177	176	5	9	6.6	34144	PASS

Average of 13.757 to 13.764 min.: VL039919.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7079	44.00	4182	52.80	75	64.90	12
37.05	47675	45.10	8922	55.05	2450	65.20	26
38.10	41216	45.90	134	56.10	14328	66.30	10
39.10	18096	46.20	385	57.05	29941	66.90	91
39.95	100	47.10	7995	58.05	1486	67.05	2205
40.30	271	48.00	5241	58.70	60	68.05	102096
40.80	80	49.00	37740	60.10	8175	69.10	105312
41.30	66	50.10	198229	61.10	42560	70.15	8766
42.00	88	51.05	61643	62.10	43597	70.85	315
42.15	115	52.00	2113	63.10	38187	71.20	454
43.05	219	52.20	1340	64.05	3731	72.00	4657

Average of 13.757 to 13.764 min.: VL039919.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	39179	83.30	140	94.10	107027	109.95	694
74.05	160000	85.20	72	95.10	863403	110.95	1217
75.10	491861	85.80	330	96.10	60875	112.00	313
76.15	41915	86.10	661	97.15	2339	112.80	1450
77.10	4740	87.05	28301	98.20	181	114.00	59
78.15	1909	88.05	25587	103.05	423	114.80	138
79.00	27891	88.80	365	103.80	1076	115.05	528
80.00	8124	90.80	1047	104.05	2665	115.90	795
81.00	27352	91.10	2422	104.95	1149	116.05	2083
82.00	5591	92.10	24464	105.95	4357	117.05	5080
82.95	544	93.10	40040	106.95	1237	118.00	3041

Average of 13.757 to 13.764 min.: VL039919.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.05	5145	128.00	2170	136.60	219	142.05	1008
119.80	112	128.20	1263	136.80	385	142.80	2236
120.00	133	129.10	1466	137.05	1167	143.15	7227
121.90	51	130.00	2766	137.90	53	143.95	843
122.10	82	130.70	398	138.30	88	144.70	264
122.80	159	131.00	656	139.00	68	145.05	589
123.70	109	132.05	275	139.25	284	145.90	499
123.95	383	133.75	153	139.80	404	146.15	722
124.70	52	134.10	252	140.20	293	146.80	489
126.10	356	135.05	1703	141.05	7759	147.95	1374
127.00	165	136.05	360	141.80	194	148.80	274

Average of 13.757 to 13.764 min.: VL039919.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.00	173	156.25	243	169.30	572	176.10	518016
149.80	339	157.05	1757	170.60	236	177.05	34144
149.95	654	157.90	66	171.10	306	178.00	1369
151.40	144	158.10	125	171.30	281	183.90	74
151.90	173	159.00	414	171.80	590	196.50	60
152.80	512	159.20	218	172.10	473	204.60	54
153.10	117	160.70	181	172.30	756	206.70	117
153.80	351	161.10	561	172.80	1091	207.25	211
154.10	266	166.70	65	173.10	3845	216.60	91
155.05	2239	167.00	129	174.10	536256	217.20	130
156.00	84	168.70	314	175.05	38992	226.10	64

Average of 13.757 to 13.764 min.: VL039919.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
281.25	157						
281.80	87						