

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL112420\
 Data File : VL036019.D
 Acq On : 25 Nov 2020 7:24
 Operator : SY/AP
 Sample : L4843-02 2X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SVP-02

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.848	3	19	50	rBV	1756824	3814618	10.65%	0.733%
2	2.996	50	65	112	rVV5	14467751	35819493	100.00%	6.885%
3	3.179	112	122	145	rVV2	10280784	20540851	57.35%	3.948%
4	3.282	145	154	161	rVV	6703170	11442128	31.94%	2.199%
5	3.330	161	169	181	rVV	15459684	32429546	90.54%	6.233%
6	3.378	181	184	203	rVV3	4015794	8153048	22.76%	1.567%
7	3.465	203	211	242	rVB	1978804	3754395	10.48%	0.722%
8	3.693	270	282	313	rBV	3518991	6428323	17.95%	1.236%
9	3.851	313	331	363	rVV	15769462	35012022	97.75%	6.729%
10	3.986	363	373	386	rVV	4434272	8079649	22.56%	1.553%
11	4.057	386	395	402	rVV	3967798	6996908	19.53%	1.345%
12	4.108	402	411	428	rVV	13675366	28749139	80.26%	5.526%
13	4.185	428	435	456	rVV	2646436	5493355	15.34%	1.056%
14	4.285	456	466	474	rVV	1817333	3400327	9.49%	0.654%
15	4.346	476	485	515	rVB2	1390449	3153585	8.80%	0.606%
16	4.533	529	543	545	rBV	462518	715175	2.00%	0.137%
17	4.565	545	553	572	rVB2	577575	1536294	4.29%	0.295%
18	4.873	623	649	651	rBV2	2093417	3777899	10.55%	0.726%
19	4.902	651	658	687	rVV	3670330	8291289	23.15%	1.594%
20	5.037	687	700	707	rVV4	4043643	8395018	23.44%	1.614%
21	5.089	707	716	751	rVV	8911702	21214472	59.23%	4.078%
22	5.353	780	798	813	rBV	8148115	18598019	51.92%	3.575%
23	5.439	813	825	858	rVB5	4996813	13610220	38.00%	2.616%
24	5.668	874	896	914	rBV2	10053278	28622126	79.91%	5.501%
25	5.751	914	922	932	rVV	1633618	3829384	10.69%	0.736%
26	5.799	932	937	954	rVV2	550285	1143624	3.19%	0.220%
27	5.899	954	968	977	rVV4	836401	1930076	5.39%	0.371%
28	5.960	977	987	1017	rVV2	1763447	3882319	10.84%	0.746%
29	6.092	1017	1028	1047	rVV3	428805	864907	2.41%	0.166%
30	6.301	1077	1093	1128	rBV6	1067746	3813835	10.65%	0.733%
31	6.487	1128	1151	1181	rVV2	6955694	16373339	45.71%	3.147%
32	6.626	1181	1194	1207	rVV4	658458	1536631	4.29%	0.295%
33	6.709	1207	1220	1237	rVV2	820170	1887828	5.27%	0.363%
34	6.819	1237	1254	1265	rVV6	2526131	6304750	17.60%	1.212%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL112420\
 Data File : VL036019.D
 Acq On : 25 Nov 2020 7:24
 Operator : SY/AP
 Sample : L4843-02 2X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SVP-02

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020

35	6.864	1265	1268	1276	rVV	726256	1213156	3.39%	0.233%
36	6.918	1276	1285	1289	rVV2	786897	1565166	4.37%	0.301%
37	6.957	1289	1297	1307	rVV4	1244500	2892160	8.07%	0.556%
38	7.021	1307	1317	1333	rVV	1495349	3457769	9.65%	0.665%
39	7.150	1333	1357	1368	rVV	6494872	15452810	43.14%	2.970%
40	7.230	1368	1382	1395	rVV4	4103749	11524232	32.17%	2.215%
41	7.307	1395	1406	1428	rVV2	1863019	4571395	12.76%	0.879%
42	7.465	1430	1455	1475	rVV	5785102	14189716	39.61%	2.727%
43	7.558	1475	1484	1509	rVB2	471896	1104014	3.08%	0.212%
44	7.725	1513	1536	1547	rBV3	1645864	5464099	15.25%	1.050%
45	7.790	1547	1556	1599	rVB2	1999503	7034385	19.64%	1.352%
46	8.037	1620	1633	1639	rBV3	224120	430067	1.20%	0.083%
47	8.102	1639	1653	1682	rVV	4001132	10878193	30.37%	2.091%
48	8.224	1682	1691	1705	rVB2	407116	848740	2.37%	0.163%
49	8.349	1716	1730	1750	rVB6	478708	1401392	3.91%	0.269%
50	8.465	1750	1766	1793	rVB3	784622	1828638	5.11%	0.351%
51	8.745	1843	1853	1859	rBV4	270638	572215	1.60%	0.110%
52	8.796	1859	1869	1906	rVB3	943796	2548430	7.11%	0.490%
53	9.021	1926	1939	1949	rBV2	294781	622936	1.74%	0.120%
54	9.095	1949	1962	1987	rVB4	1080334	2845782	7.94%	0.547%
55	9.333	2022	2036	2048	rBV4	172808	426895	1.19%	0.082%
56	9.446	2048	2071	2080	rVV4	722856	2135888	5.96%	0.411%
57	9.513	2080	2092	2107	rVV2	1416163	4144726	11.57%	0.797%
58	9.590	2107	2116	2134	rVV5	605427	1854328	5.18%	0.356%
59	9.693	2134	2148	2149	rVV3	588505	872190	2.43%	0.168%
60	9.729	2153	2159	2168	rVV3	643913	1546095	4.32%	0.297%
61	9.774	2168	2173	2184	rVV2	507878	1042937	2.91%	0.200%
62	9.896	2199	2211	2218	rVV3	521845	1214917	3.39%	0.234%
63	9.947	2218	2227	2240	rVV3	706260	1683234	4.70%	0.324%
64	10.031	2240	2253	2263	rVV2	1301797	3149680	8.79%	0.605%
65	10.085	2263	2270	2285	rVV4	756866	1674290	4.67%	0.322%
66	10.185	2285	2301	2313	rVV3	458960	1115993	3.12%	0.214%
67	10.272	2313	2328	2339	rVV2	1869684	4816345	13.45%	0.926%
68	10.310	2339	2340	2357	rVV2	835327	1285065	3.59%	0.247%
69	10.410	2357	2371	2377	rVV10	179871	517530	1.44%	0.099%
70	10.462	2377	2387	2399	rVB6	240596	607204	1.70%	0.117%
71	10.587	2414	2426	2439	rBV3	367414	815468	2.28%	0.157%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL112420\
 Data File : VL036019.D
 Acq On : 25 Nov 2020 7:24
 Operator : SY/AP
 Sample : L4843-02 2X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SVP-02

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 3 Min Area: 3 % of largest Peak
 Start Thrs: 0.001 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

72	10.664	2439	2450	2455	rVV5	342836	721630	2.01%	0.139%
73	10.709	2455	2464	2490	rVB5	649833	1835404	5.12%	0.353%
74	11.060	2553	2573	2592	rBV4	1097158	2882619	8.05%	0.554%
75	11.445	2692	2693	2716	rVB7	215513	449345	1.25%	0.086%
76	11.802	2790	2804	2820	rVB6	157513	406087	1.13%	0.078%
77	12.060	2869	2884	2910	rVV2	5798252	14352835	40.07%	2.759%
78	12.201	2910	2928	2950	rVV6	276528	1229816	3.43%	0.236%
79	12.326	2953	2967	2979	rVB3	251181	612974	1.71%	0.118%
80	12.516	3014	3026	3037	rBV5	176646	453046	1.26%	0.087%
81	12.950	3140	3161	3163	rVV6	205134	486368	1.36%	0.093%
82	12.960	3163	3164	3181	rVV6	200731	378877	1.06%	0.073%
83	13.063	3181	3196	3214	rVB6	239572	736858	2.06%	0.142%
84	13.291	3244	3267	3286	rBV4	285721	876600	2.45%	0.168%
85	14.391	3591	3609	3650	rBV	5865755	14968187	41.79%	2.877%
86	15.294	3874	3890	3907	rVB3	397193	945277	2.64%	0.182%


Sum of corrected areas: 520278595

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL112420\
Data File : VL036019.D
Acq On : 25 Nov 2020 7:24
Operator : SY/AP
Sample : L4843-02 2X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SVP-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

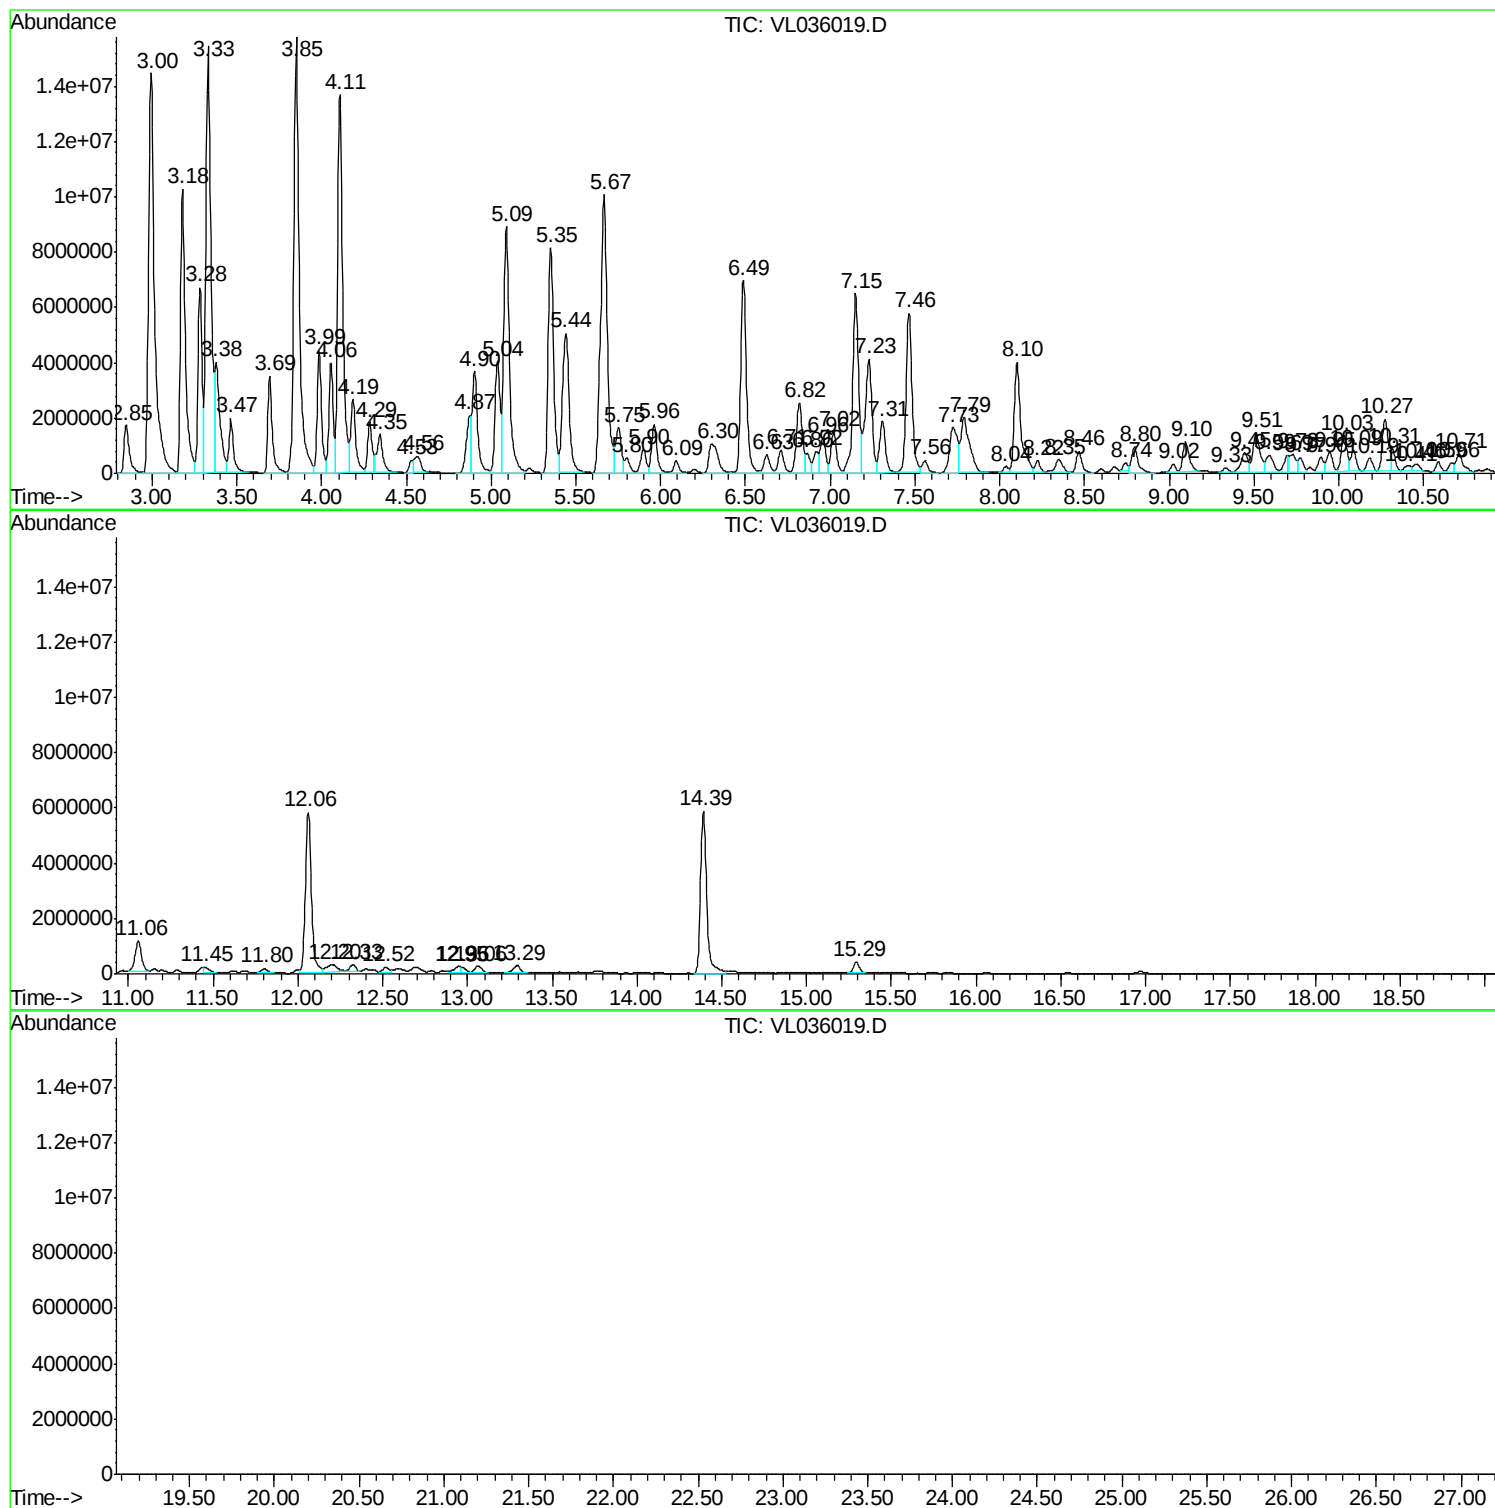

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL112420\
Data File : VL036019.D
Acq On : 25 Nov 2020 7:24
Operator : SY/AP
Sample : L4843-02 2X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SVP-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL112420\
Data File : VL036019.D
Acq On : 25 Nov 2020 7:24
Operator : SY/AP
Sample : L4843-02 2X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SVP-02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL110320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 04 02:40:06 2020

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc