

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112425\
 Data File : VL043290.D
 Acq On : 25 Nov 2025 08:21
 Operator : SY/MD
 Sample : QC112425 CAN 10315
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC112425 CAN 10315

Quant Time: Nov 26 00:10:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Nov 19 01:11:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	109733	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	274585	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.872	117	212841	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.370	95	147790	9.473	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112425\
Data File : VL043290.D
Acq On : 25 Nov 2025 08:21
Operator : SY/MD
Sample : QC112425 CAN 10315
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC112425 CAN 10315

Quant Time: Nov 26 00:10:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed Nov 19 01:11:25 2025
Response via : Initial Calibration




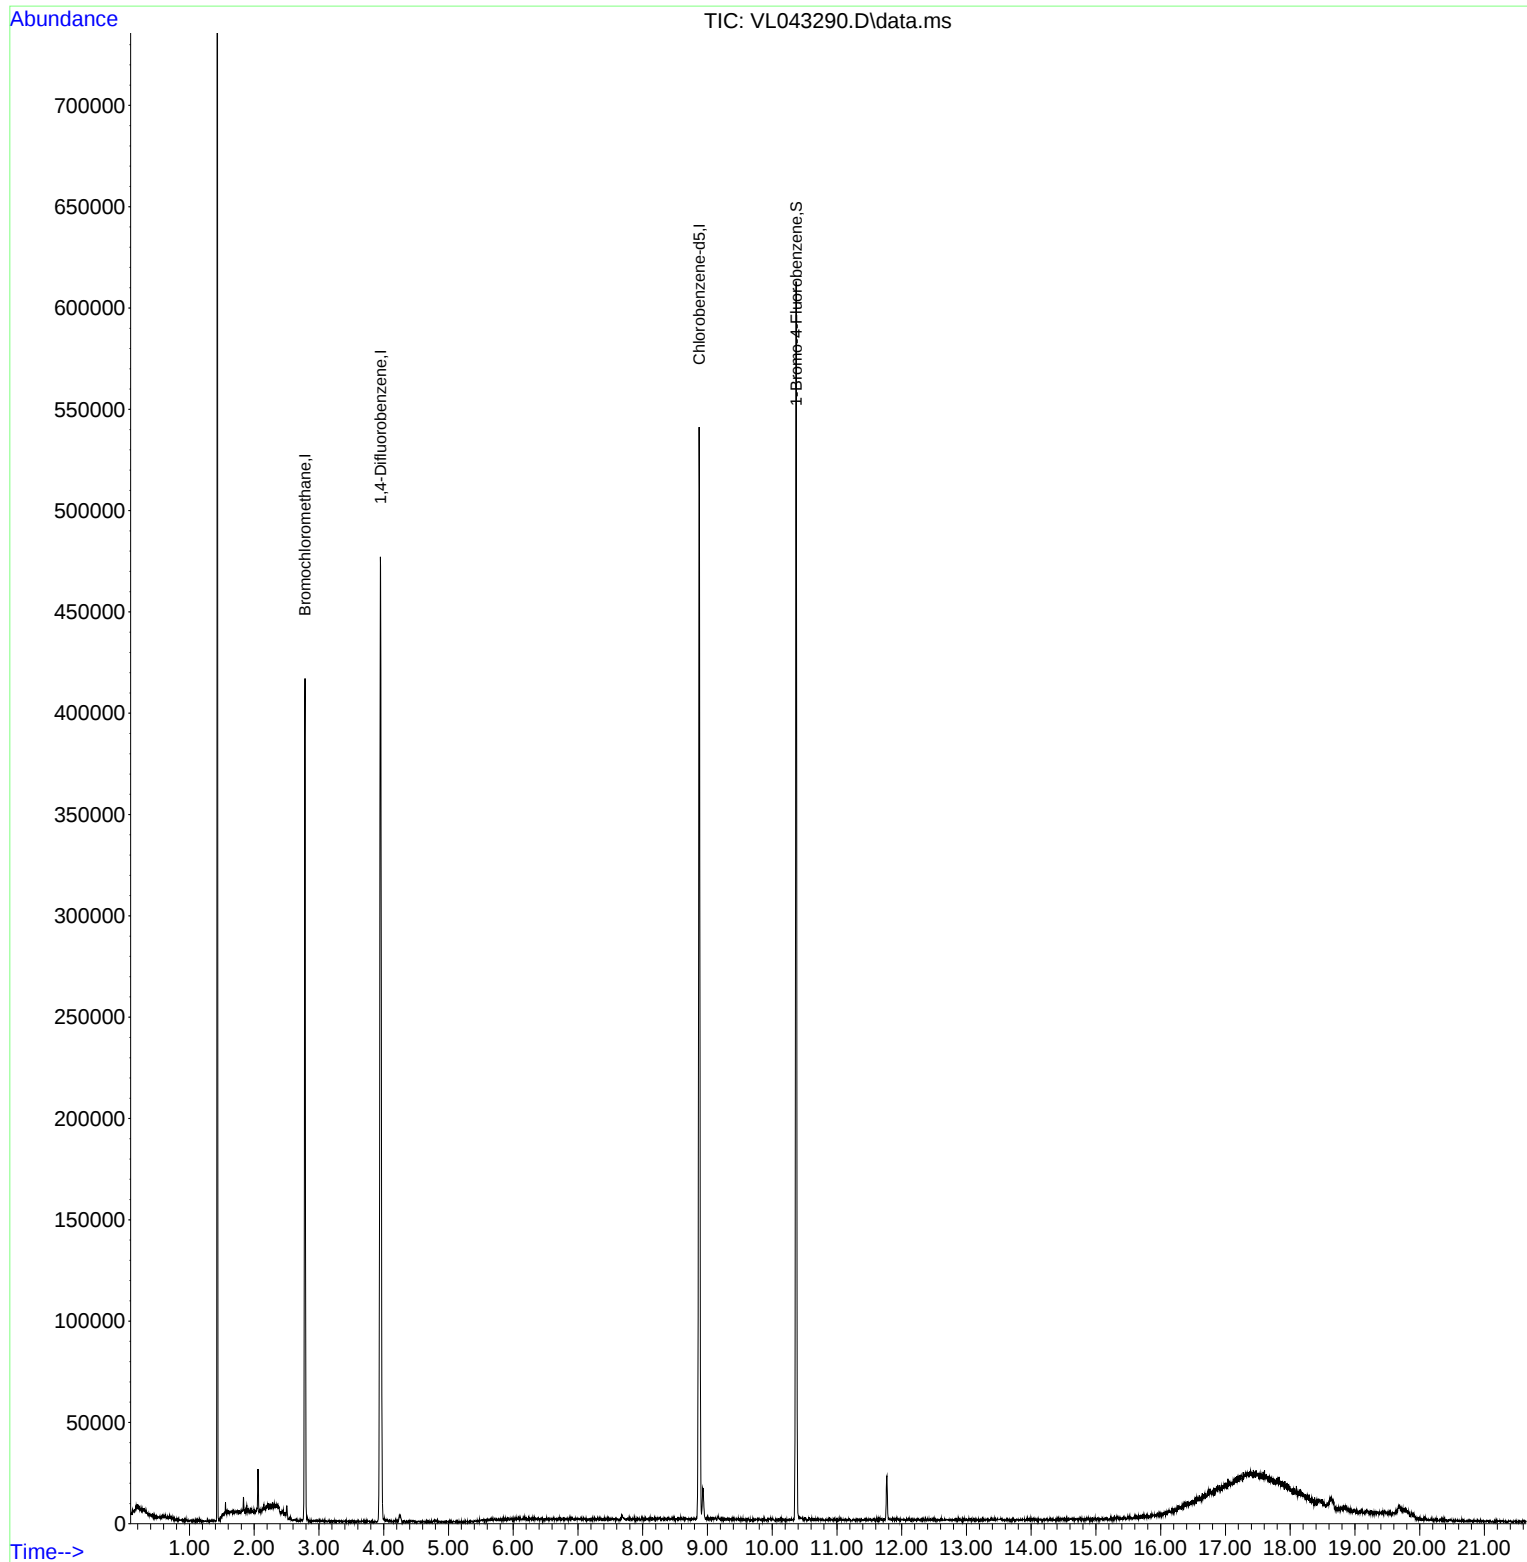


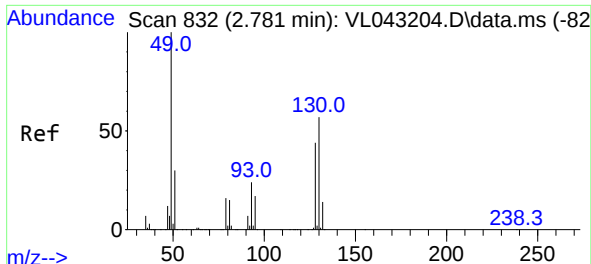

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.784 min Scan# 81
Delta R.T. 0.003 min
Lab File: VL043290.D
Acq: 25 Nov 2025 08:21




Instrument :
MSVOA_L
ClientSampleId :
QC112425 CAN 10315


Tgt Ion: 49 Resp: 109733
Ion Ratio Lower Upper
49 100
128 49.3 23.0 69.0
130 63.3 29.9 89.7

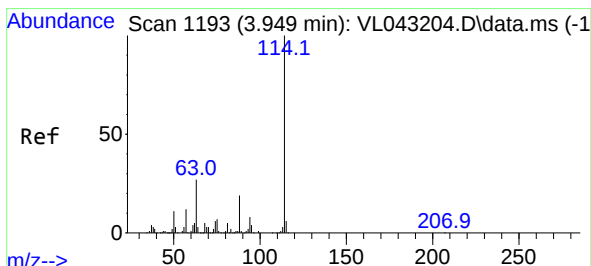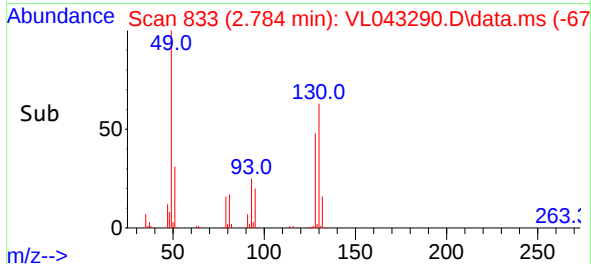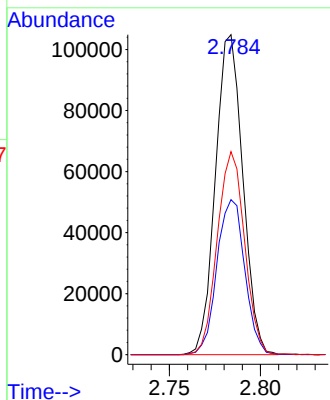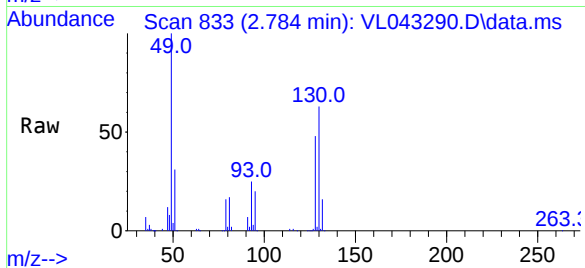

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.952 min Scan# 1194
Delta R.T. 0.003 min
Lab File: VL043290.D
Acq: 25 Nov 2025 08:21

Tgt Ion: 114 Resp: 274585
Ion Ratio Lower Upper
114 100
63 26.0 21.0 31.6
88 18.6 14.9 22.3


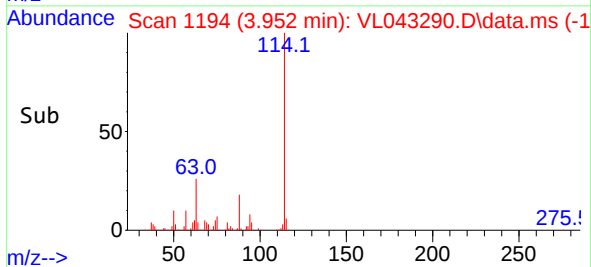
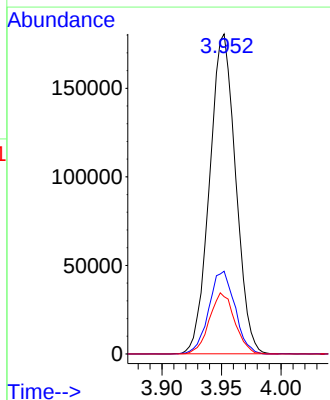
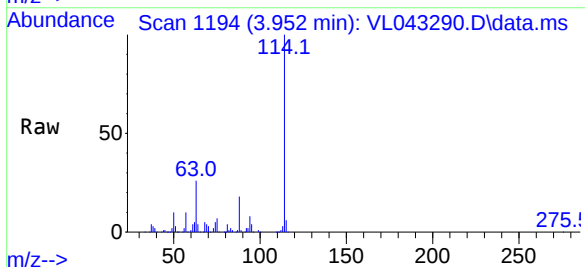


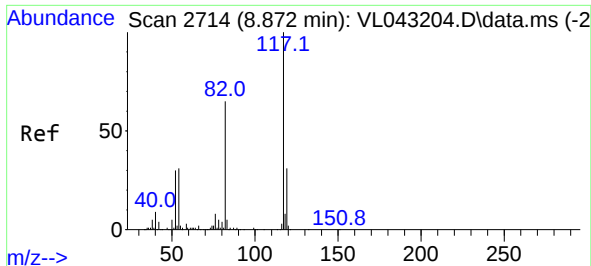

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.872 min Scan# 21
Delta R.T. -0.000 min
Lab File: VL043290.D
Acq: 25 Nov 2025 08:21

Instrument :
MSVOA_L
ClientSampleId :
QC112425 CAN 10315

Tgt Ion:117 Resp: 212841
Ion Ratio Lower Upper
117 100
82 65.7 56.1 84.1
119 31.7 25.0 37.6

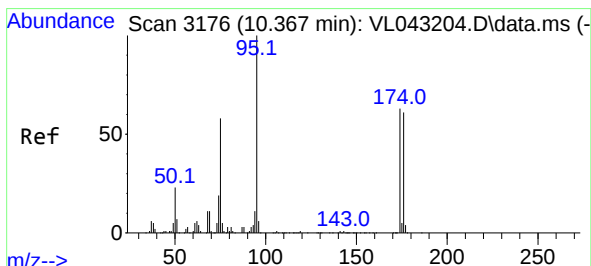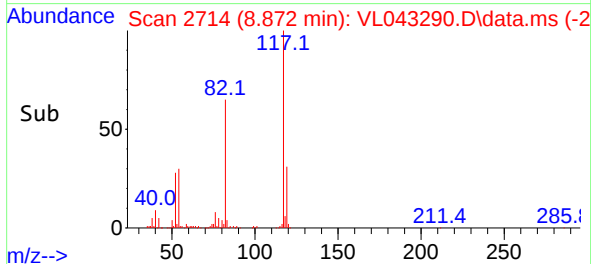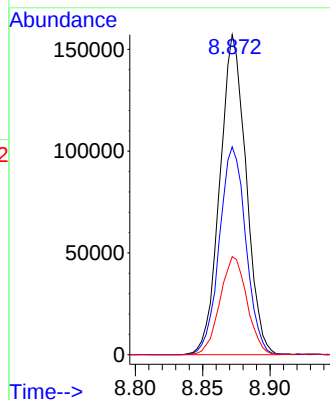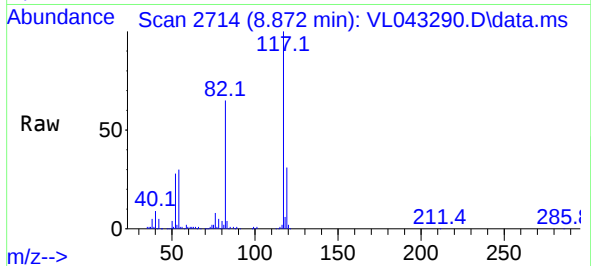

#68
1-Bromo-4-Fluorobenzene
Concen: 9.473 ppbv
RT: 10.370 min Scan# 3177
Delta R.T. 0.003 min
Lab File: VL043290.D
Acq: 25 Nov 2025 08:21

Tgt Ion: 95 Resp: 147790
Ion Ratio Lower Upper
95 100
174 66.1 50.2 75.2
175 4.9 4.1 6.1

