
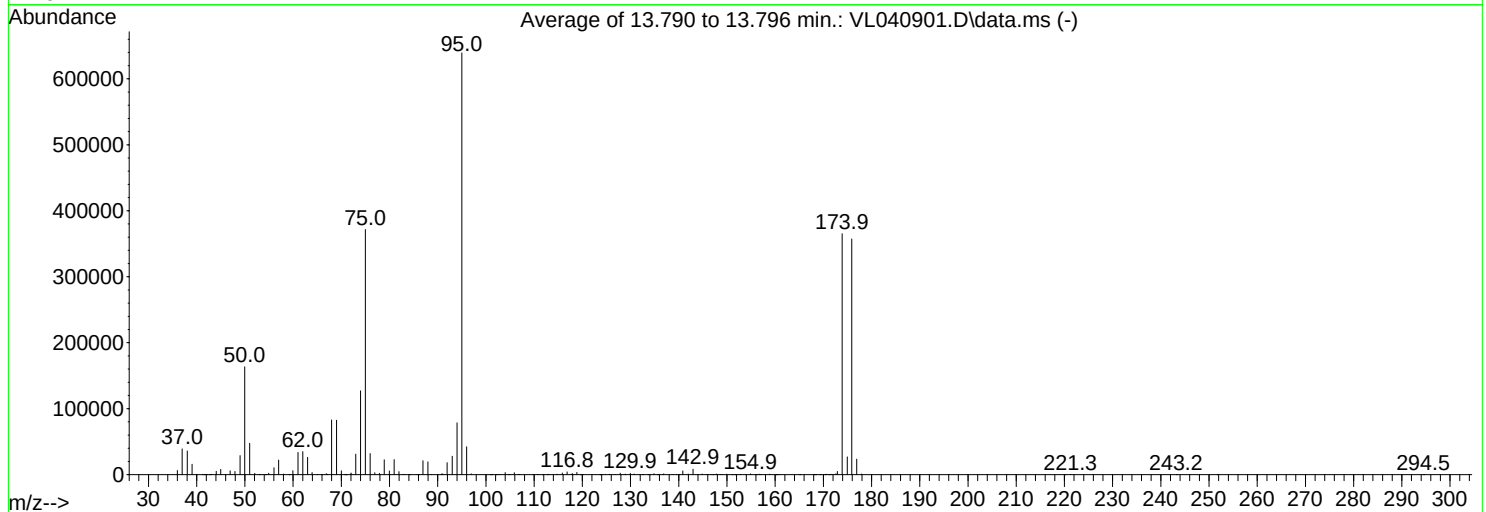


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112723\
 Data File : VL040901.D
 Acq On : 27 Nov 2023 8:34
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111323AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Nov 28 04:31:59 2023

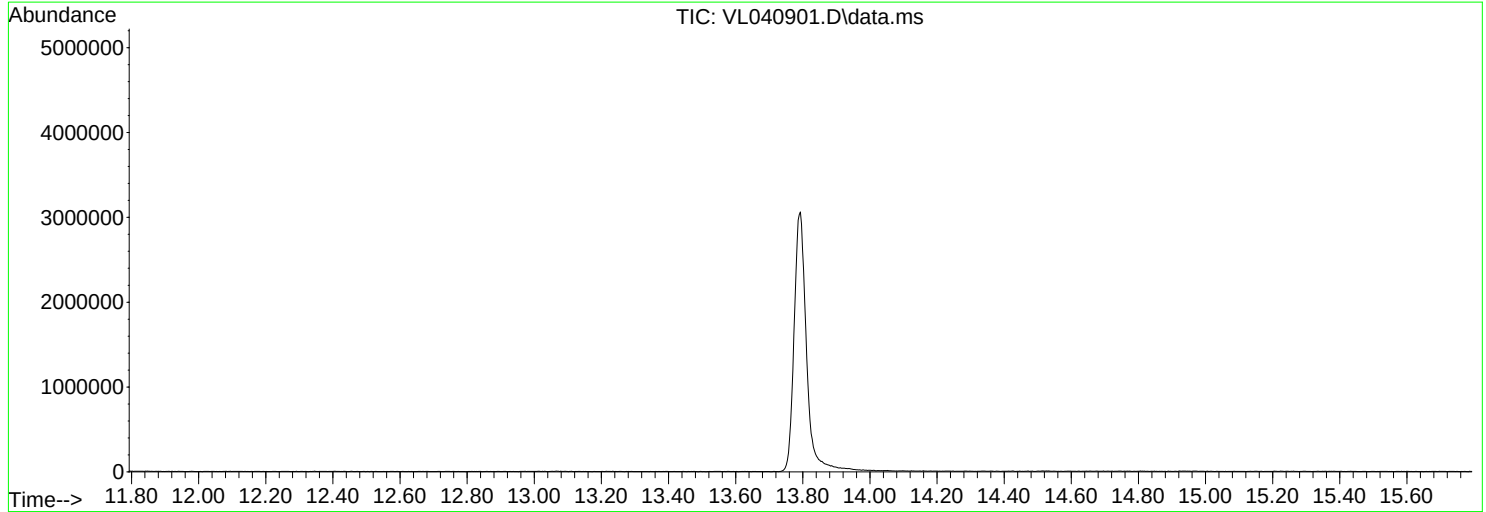

AutoFind: Scans 3479, 3480, 3481; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.6	163419	PASS
75	95	30	66	58.1	371584	PASS
95	95	100	100	100.0	639403	PASS
96	95	5	9	6.6	42208	PASS
173	174	0.00	2	1.3	4827	PASS
174	95	50	120	57.1	365397	PASS
175	174	4	9	7.4	26904	PASS
176	174	93	101	97.8	357397	PASS
177	176	5	9	6.6	23667	PASS

Average of 13.790 to 13.796 min.: VL040901.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6325	45.00	7982	54.95	2110	65.90	50
37.00	39136	46.00	576	56.05	10369	66.90	145
38.05	36019	46.95	5858	57.00	22099	67.10	52
39.05	15789	47.95	4873	58.05	1064	68.00	8308
40.05	623	49.00	28781	59.20	65	69.00	82413
41.20	76	49.95	163419	59.95	6109	70.00	5864
41.60	93	51.00	47635	61.00	33707	70.70	124
42.00	50	52.05	2052	62.00	34936	71.00	77
42.70	136	53.00	145	63.00	26237	71.90	1058
43.10	416	53.70	182	63.95	3291	72.05	2340
44.05	5128	54.30	84	65.05	519	73.00	31085

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 13.790 to 13.796 min.: VL040901.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	127195	84.10	60	94.00	78661	104.80	239
75.00	371584	85.70	263	95.00	639403	104.95	395
76.00	32115	86.00	222	96.00	42208	105.90	3020
76.95	2896	86.20	319	96.95	1153	106.75	550
77.90	2003	86.95	20997	100.90	103	107.00	267
78.90	22635	87.95	19320	101.20	88	109.85	501
79.95	5708	88.70	310	102.10	83	110.10	291
80.95	22909	90.80	1103	102.60	171	110.70	239
81.95	4594	91.05	1201	102.90	318	110.95	349
82.80	422	91.95	18104	104.00	3067	111.70	101
83.15	301	93.00	27984	104.70	283	112.00	429

Average of 13.790 to 13.796 min.: VL040901.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
112.70	142	123.60	81	131.90	233	140.10	254
113.05	456	123.80	101	132.50	57	140.85	5600
114.75	737	124.10	203	133.60	138	141.95	1023
115.85	2432	124.75	432	134.10	168	142.95	8270
116.85	4102	125.65	417	134.85	1362	143.95	353
117.80	652	126.80	265	135.60	99	144.85	1049
117.95	1589	127.85	2237	135.95	166	145.85	536
118.85	3426	128.70	341	136.70	342	146.10	273
119.60	132	128.95	693	136.90	1153	146.80	297
120.20	202	129.95	2077	138.80	212	147.10	86
122.80	258	130.75	1111	139.50	349	147.80	895

Average of 13.790 to 13.796 min.: VL040901.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.00	308	156.10	5	168.40	70	174.95	26904
148.60	210	156.70	683	169.30	53	175.90	357397
149.00	255	157.05	598	170.30	57	176.90	23667
149.90	847	157.90	228	170.70	727	177.90	881
151.10	151	158.90	846	171.10	151	220.10	56
151.70	145	160.10	70	171.50	234	221.30	168
151.90	142	160.30	65	171.65	568	243.20	77
152.75	433	160.75	349	172.00	324	251.70	66
153.95	252	161.00	246	172.60	1264	294.50	99
154.90	1179	165.10	146	172.90	4827		
155.80	99	168.10	72	173.90	365397		