


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL113018\
Data File : VL032845.D
Acq On : 30 Nov 2018 10:38
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111418AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 14 07:00:23 2018
Last Update : Wed Nov 14 07:00:23 2018

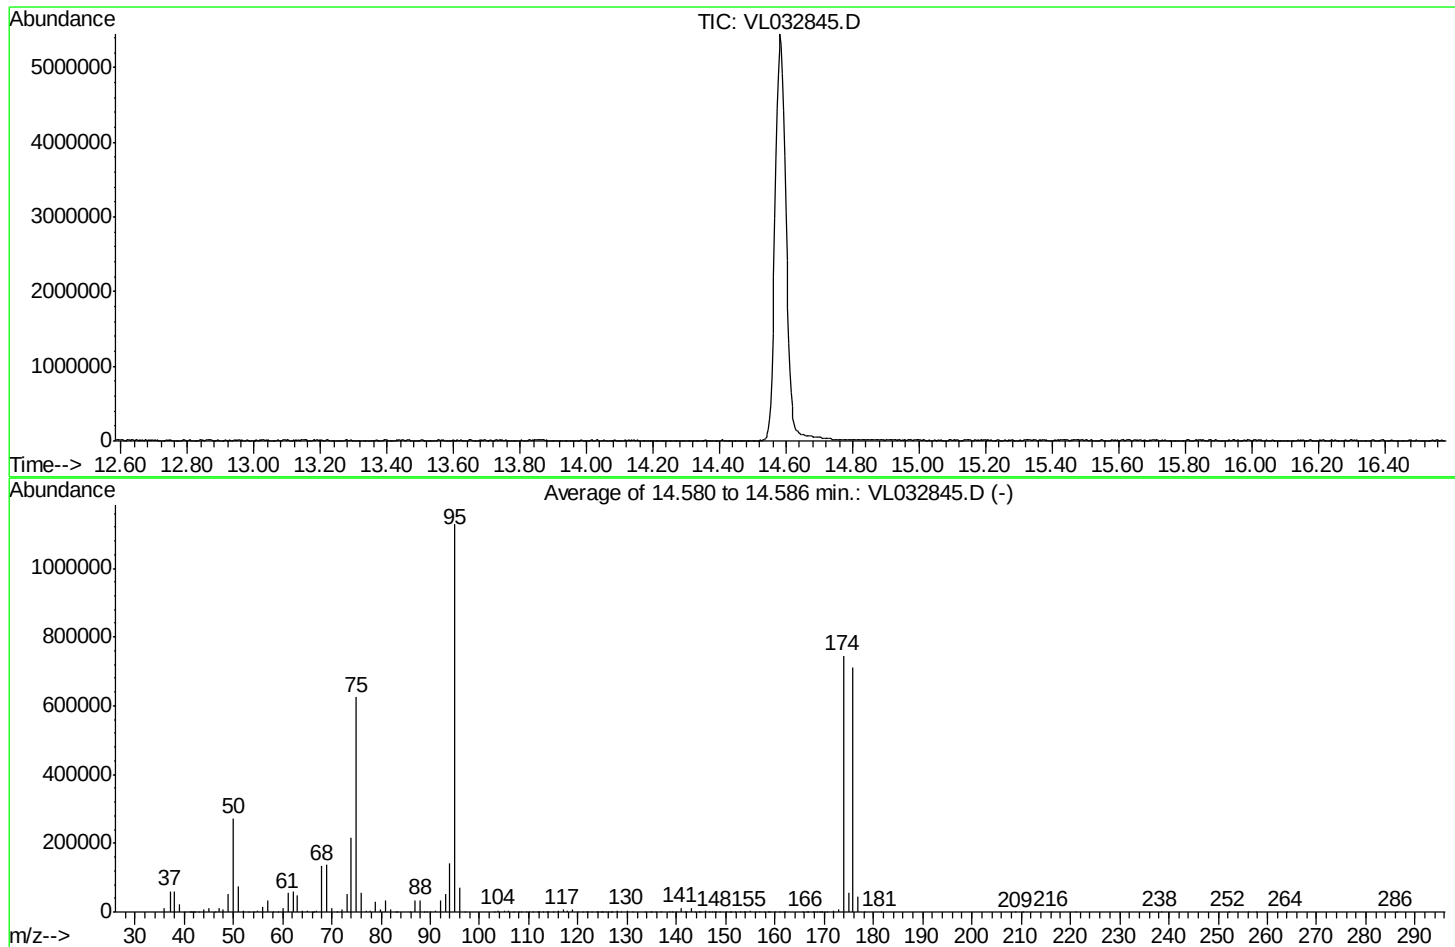

AutoFind: Scans 3621, 3622, 3623; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	271018	PASS
75	95	30	66	55.4	624618	PASS
95	95	100	100	100.0	1127936	PASS
96	95	5	9	6.4	72384	PASS
173	174	0.00	2	1.0	7240	PASS
174	95	50	120	66.1	745431	PASS
175	174	4	9	7.5	56176	PASS
176	174	93	101	95.3	710186	PASS
177	176	5	9	6.3	45008	PASS