

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL113020\
 Data File : VL036031.D
 Acq On : 30 Nov 2020 16:04
 Operator : SY/AP
 Sample : VSTDICC015
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Quant Time: Nov 30 16:35:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL113020BRAIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Nov 30 16:15:04 2020
 QLast Update : Mon Nov 30 16:15:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.71	49	1206745	10.00	ppbv	0.00
3) 1,4-Difluorobenzene	7.22	114	4063059	10.00	ppbv	0.00
4) Chlorobenzene-d5	12.14	117	3822393	10.00	ppbv	0.00

System Monitoring Compounds

5) 1-Bromo-4-Fluorobenzene	14.47	95	3018070	11.11	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	111.10%


Target Compounds					Ovalue
2) Bromomethane	3.50	94	1134174	15.758	ppbv 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL113020\
Data File : VL036031.D
Acq On : 30 Nov 2020 16:04
Operator : SY/AP
Sample : VSTDIC015
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDIC015

Quant Time: Nov 30 16:35:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL113020BRAIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Nov 30 16:15:04 2020
QLast Update : Mon Nov 30 16:15:04 2020
Response via : Initial Calibration

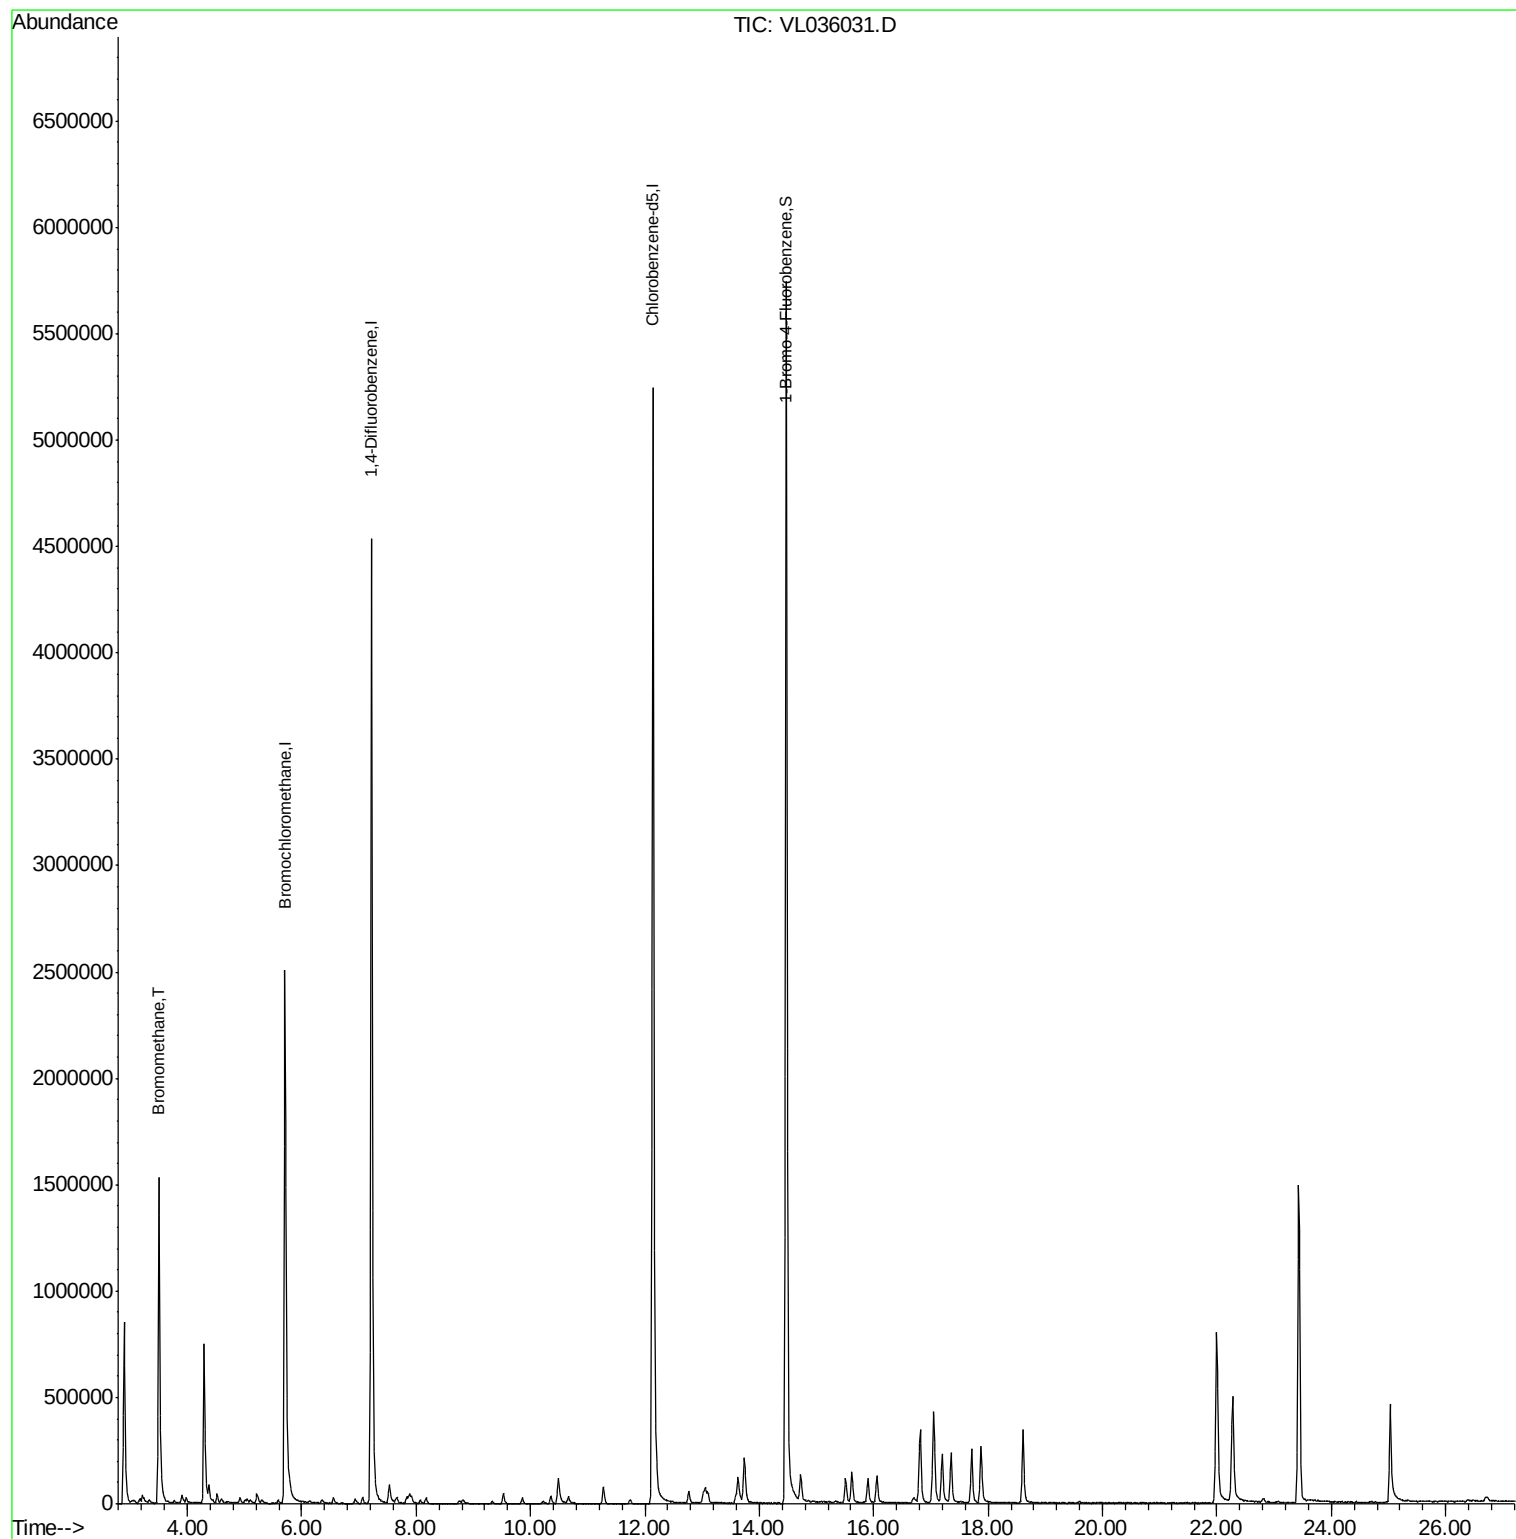

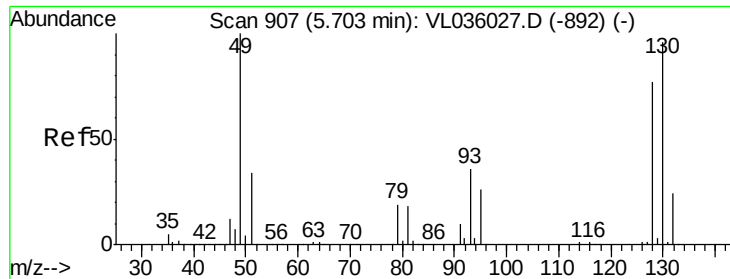

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.71 min Scan# 908

Delta R.T. 0.00 min

Lab File: VL036031.D

Acq: 30 Nov 2020 16:04

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC015


Tot Ion: 49 Resp: 1206745

Ion Ratio Lower Upper

49 100

128 74.3 38.0 114.1




130 93.9 49.2 147.6

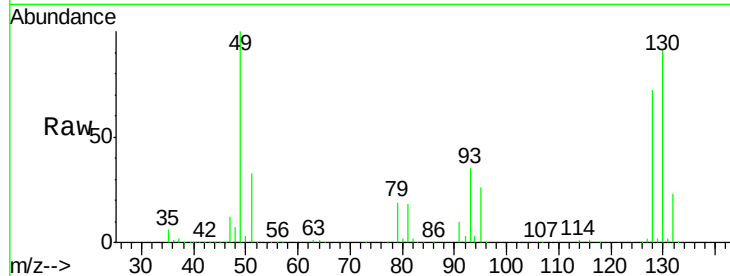

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

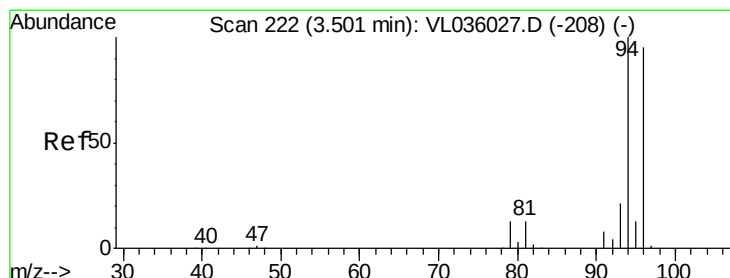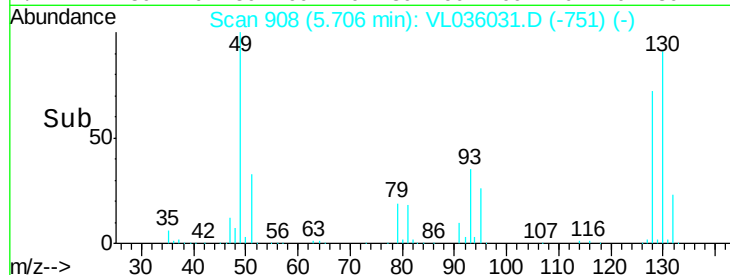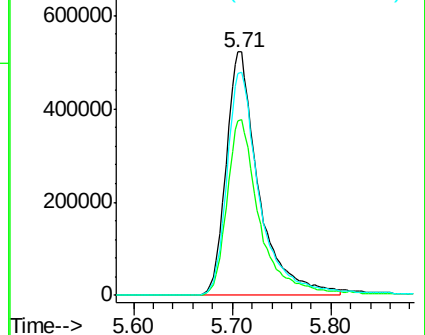

#2

Bromomethane

Concen: 15.758 ppbv

RT: 3.50 min Scan# 222

Delta R.T. -0.00 min

Lab File: VL036031.D


Acq: 30 Nov 2020 16:04

Tgt Ion: 94 Resp: 1134174

Ion Ratio Lower Upper



94 100


96 95.2 75.7 113.5

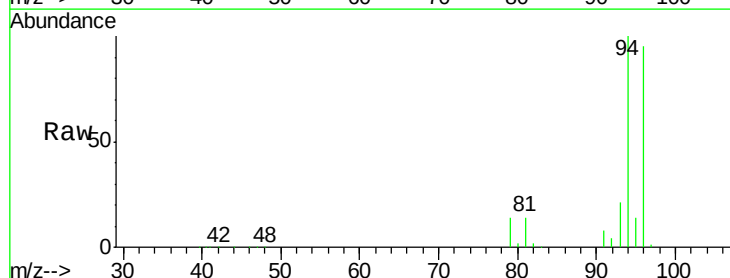

Abundance Ion 94.00 (93.70 to 94.70): VL0

Ion 96.00 (95.70 to 96.70): VL0

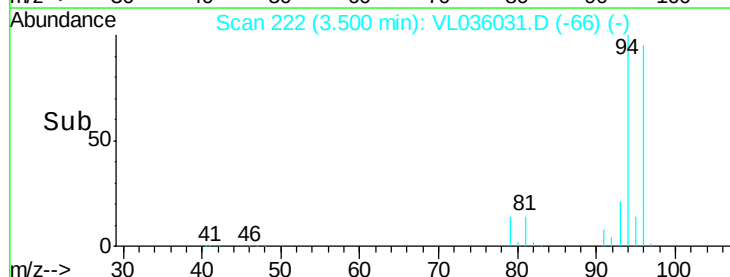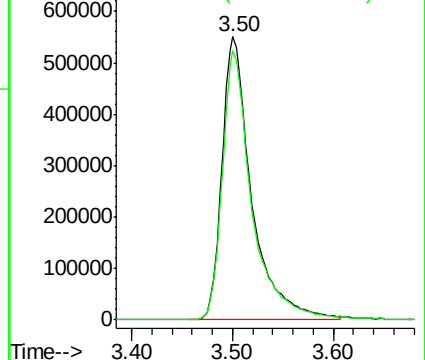

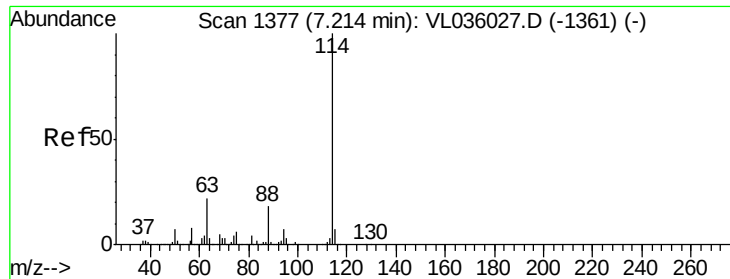

#3

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.22 min Scan# 1379

Delta R.T. 0.01 min

Lab File: VL036031.D

Acq: 30 Nov 2020 16:04

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC015


Tot Ion:114 Resp: 4063059

Ion Ratio Lower Upper

114 100

63 21.5 16.6 24.8




88 17.7 14.0 21.0

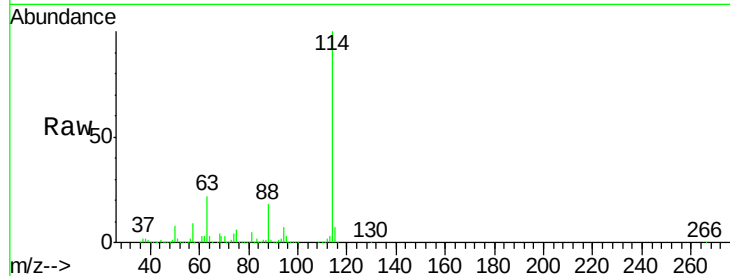

Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

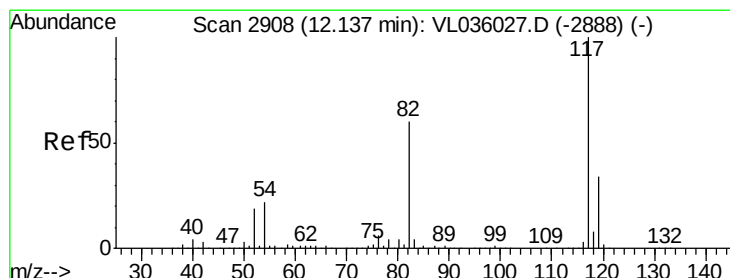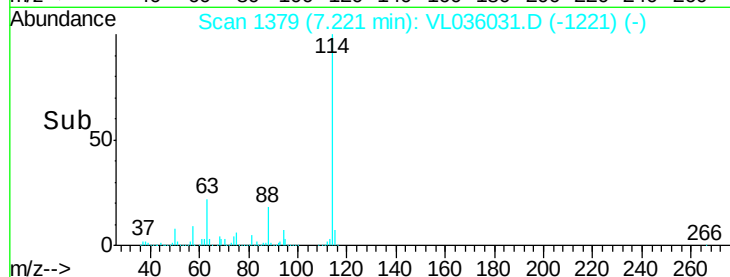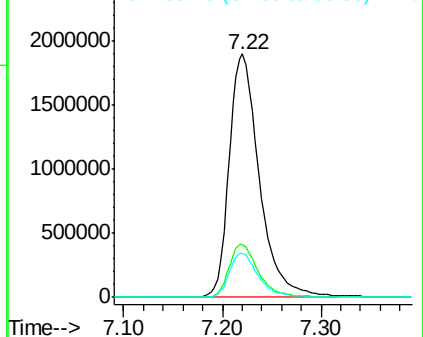

#4

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.14 min Scan# 2909

Delta R.T. 0.00 min

Lab File: VL036031.D

Acq: 30 Nov 2020 16:04


Tgt Ion:117 Resp: 3822393

Ion Ratio Lower Upper

117 100

82 62.4 48.6 73.0



119 34.1 27.5 41.3



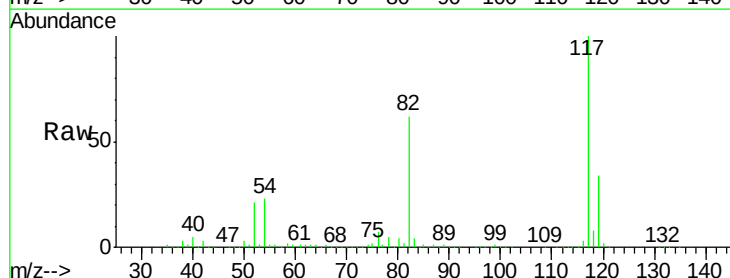


Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

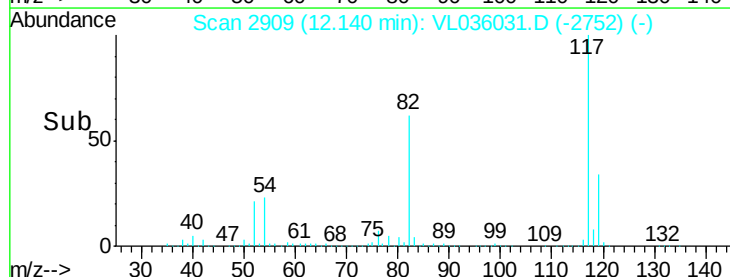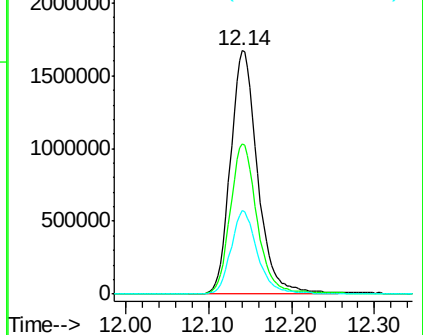

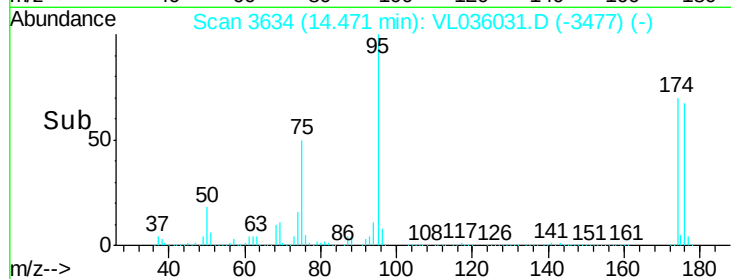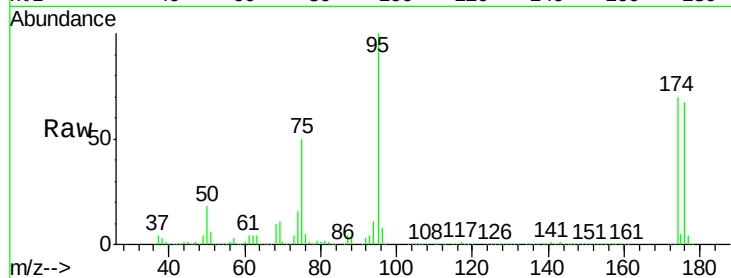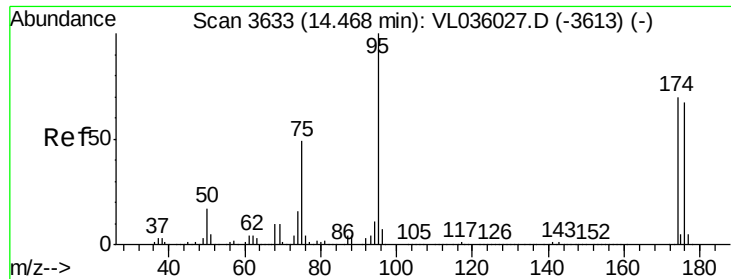

#5

1-Bromo-4-Fluorobenzene

Concen: 11.113 ppbv

RT: 14.47 min Scan# 3634

Delta R.T. 0.00 min

Lab File: VL036031.D

Acq: 30 Nov 2020 16:04

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC015

Tot Ion: 95 Resp: 3018070

Ion Ratio Lower Upper

95 100

174 69.0 56.2 84.2

175 4.9 4.0 6.0

