


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL113020\
 Data File : VL036026.D
 Acq On : 30 Nov 2020 12:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL113020BRAIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020
 Last Update : Wed Nov 04 02:40:06 2020

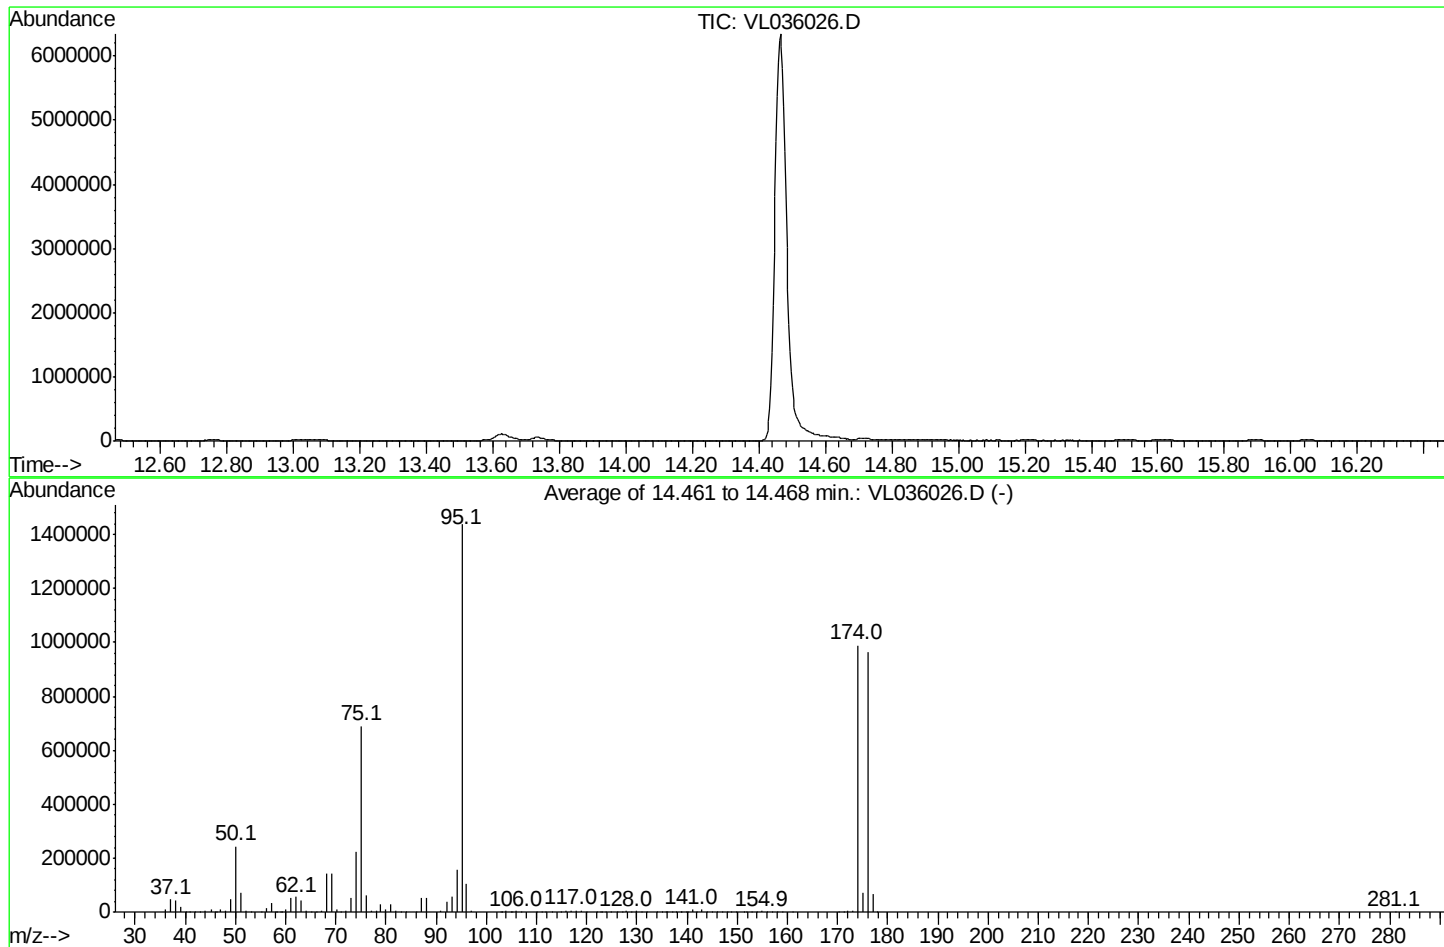

AutoFind: Scans 3631, 3632, 3633; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	16.9	243328	PASS
75	95	30	66	47.9	689365	PASS
95	95	100	100	100.0	1438549	PASS
96	95	5	9	7.2	103221	PASS
173	174	0.00	2	0.6	5520	PASS
174	95	50	120	68.8	990144	PASS
175	174	4	9	7.2	71626	PASS
176	174	93	101	97.2	962240	PASS
177	176	5	9	6.9	66234	PASS