


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL120319\
Data File : VL034452.D
Acq On : 3 Dec 2019 9:37
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111919AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Nov 19 14:15:35 2019
Last Update : Tue Nov 19 14:15:35 2019

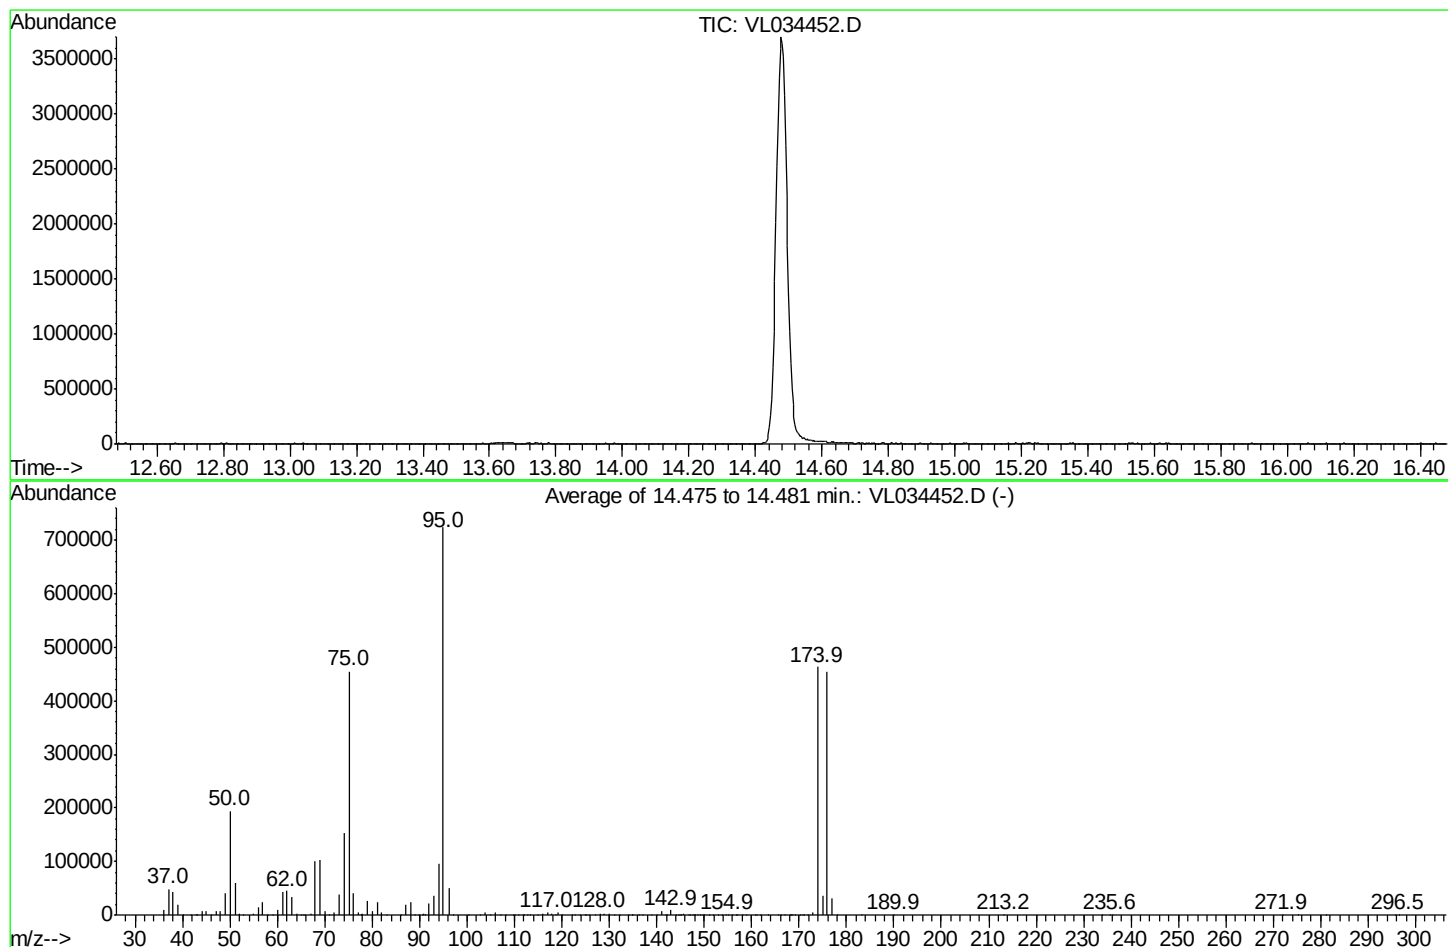

AutoFind: Scans 3635, 3636, 3637; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.9	194901	PASS
75	95	30	66	62.8	454741	PASS
95	95	100	100	100.0	723989	PASS
96	95	5	9	6.9	50240	PASS
173	174	0.00	2	0.8	3780	PASS
174	95	50	120	63.9	462677	PASS
175	174	4	9	7.7	35466	PASS
176	174	93	101	98.3	454741	PASS
177	176	5	9	7.1	32205	PASS